

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
 Data File : BP013798.D
 Acq On : 08 Feb 2023 15:48
 Operator : CG/JU
 Sample : 01422-08
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B46

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/09/2023
 Supervised By :Sohil Jodhani 02/09/2023

Quant Time: Feb 08 23:56:15 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 08 00:37:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.122	152	170568	20.000	ng/u1	0.00
20) Naphthalene-d8	10.951	136	735155	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.757	164	517526	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.510	188	1256639	20.000	ng/u1	0.00
79) Chrysene-d12	21.586	240	1262354	20.000	ng/u1	0.00
88) Perylene-d12	24.151	264	1147717	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.469	96	17662	4.292	ng/uL	0.00
4) Pyridine-d5	3.910	84	75693	6.204	ng/u1	0.00
7) Phenol-d5	7.269	99	104134	6.852	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.440	67	202698	22.761	ng/u1	0.00
11) 2-Chlorophenol-d4	7.646	132	223546	19.982	ng/u1	0.00
15) 4-Methylphenol-d8	8.828	113	169687	13.661	ng/u1	0.00
21) Nitrobenzene-d5	9.293	128	127307	24.889	ng/u1	0.00
24) 2-Nitrophenol-d4	10.022	143	137567	23.293	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.563	165	269903	22.426	ng/u1	0.00
31) 4-Chloroaniline-d4	11.081	131	290259	17.014	ng/u1	0.00
46) Dimethylphthalate-d6	14.157	166	1044399	25.622	ng/u1	0.00
49) Acenaphthylene-d8	14.457	160	1117922	25.336	ng/u1	0.00
54) 4-Nitrophenol-d4	14.939	143	42361m	5.833	ng/u1	0.00
60) Fluorene-d10	15.751	176	935118	26.934	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	128571	16.677	ng/u1	0.00
73) Anthracene-d10	17.610	188	1626424	28.305	ng/u1	0.00
81) Pyrene-d10	19.827	212	2118698	29.596	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.986	264	1715481	29.830	ng/u1	0.00
Target Compounds						
78) Di-n-butylphthalate	18.439	149	414201	5.795	ng/u1	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013798.D
Acq On : 08 Feb 2023 15:48
Operator : CG/JU
Sample : 01422-08
Misc :
ALS Vial : 13 Sample Multiplier: 1


Instrument :
BNA_P
ClientSampleId :
C0B46

Quant Time: Feb 08 23:56:15 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 08 00:37:14 2023
Response via : Initial Calibration

Manual Integrations
APPROVED


Reviewed By :Jagrut Upadhyay 02/09/2023
Supervised By :Sohil Jodhani 02/09/2023

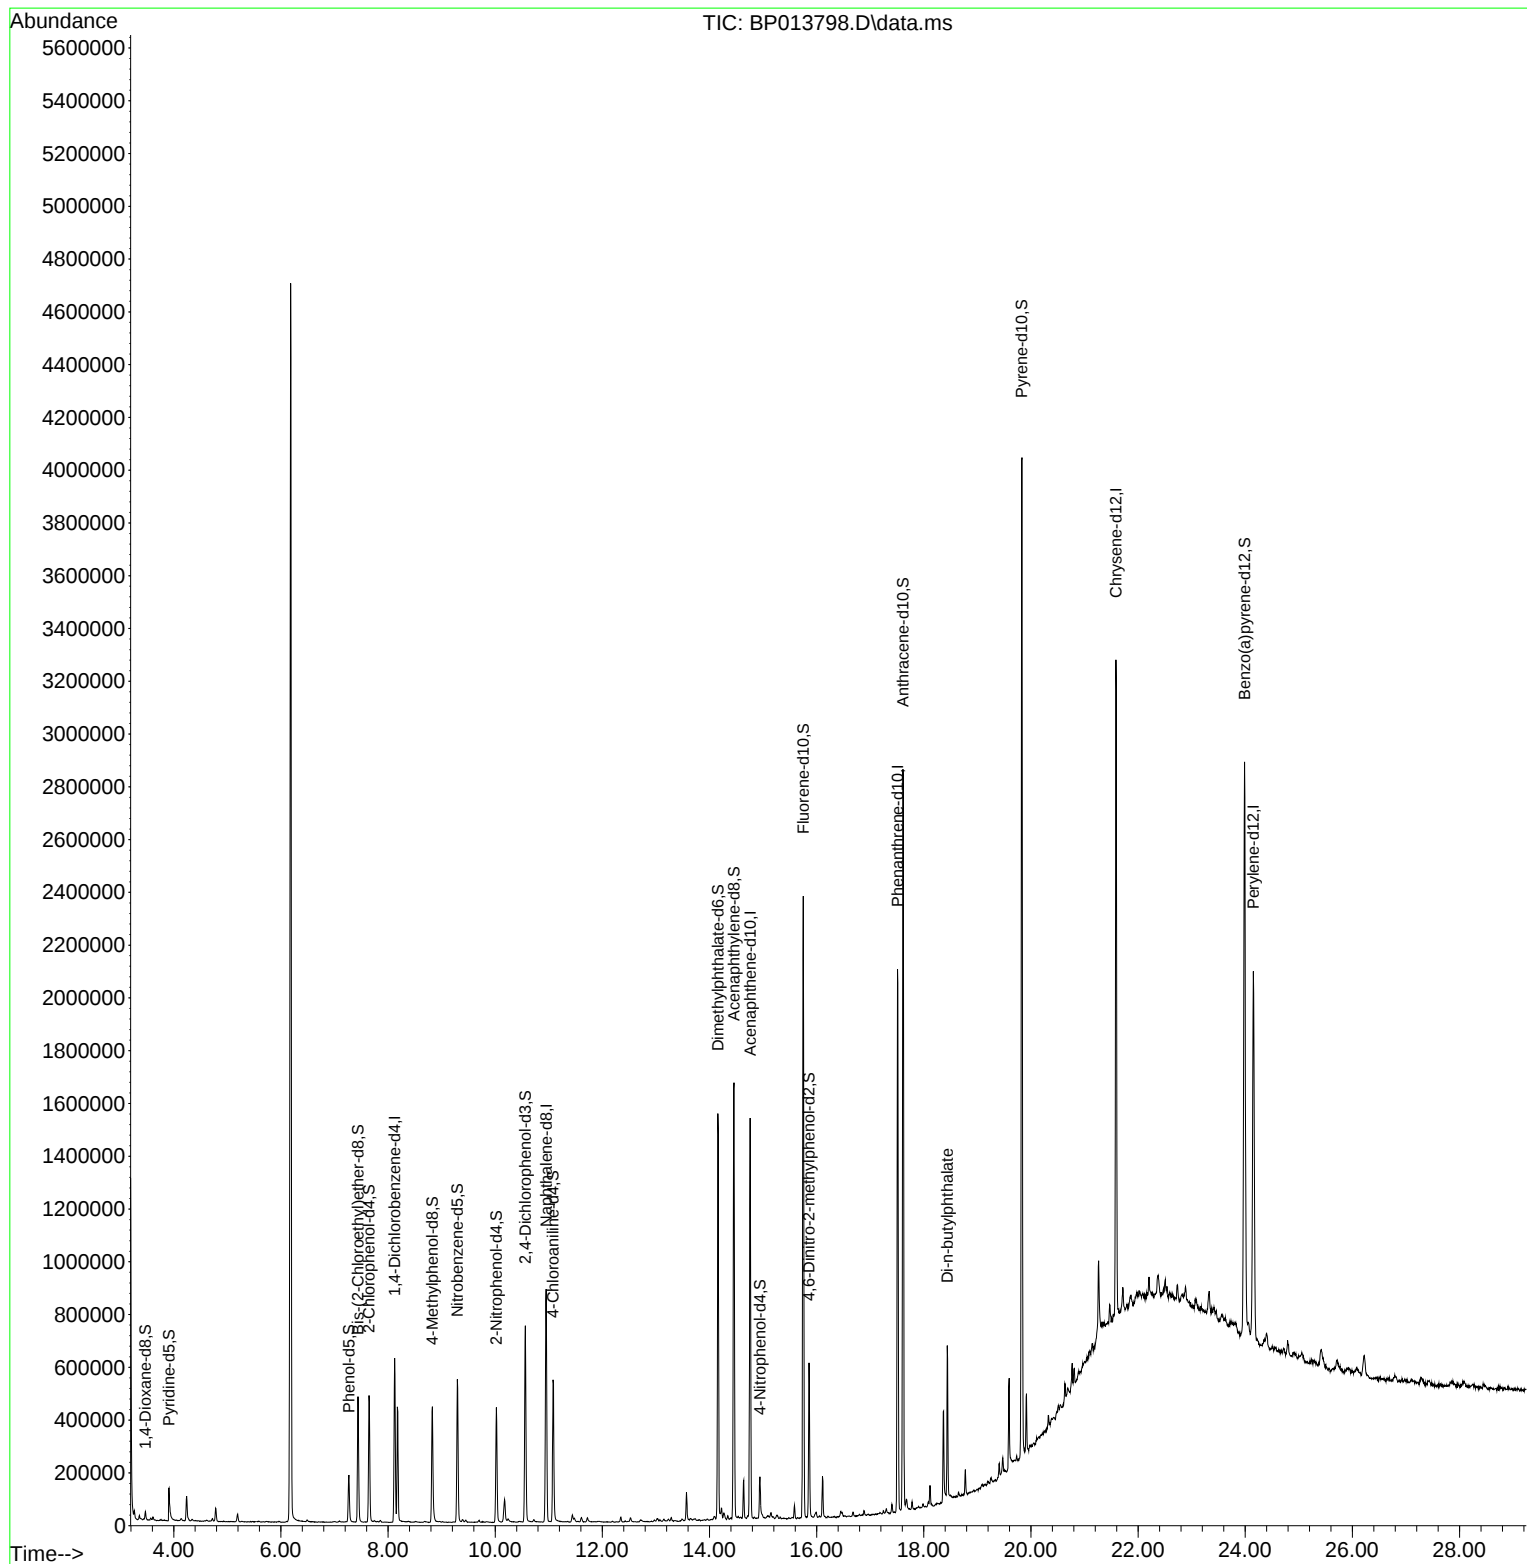

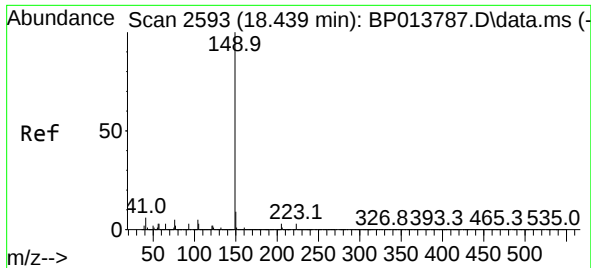

#78
 Di-n-butylphthalate
 Concen: 5.795 ng/ul
 RT: 18.439 min Scan# 2593
 Delta R.T. -0.006 min
 Lab File: BP013798.D
 Acq: 08 Feb 2023 15:48

Instrument :
 BNA_P
 ClientSampleId :
 C0B46

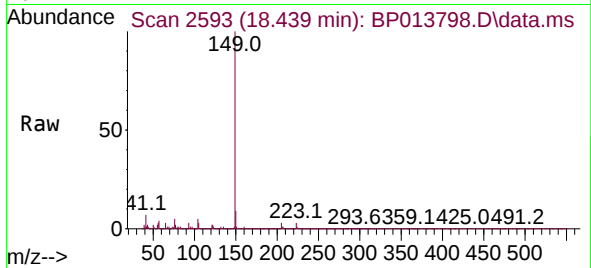

Tgt Ion:149 Resp: 414201
 Ion Ratio Lower Upper
 149 100
 150 9.2 7.1 10.7
 104 5.2 4.1 6.1

Manual Integrations
 APPROVED

Reviewed By :Jagrut Upadhyay 02/09/2023
 Supervised By :Sohil Jodhani 02/09/2023

