

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
 Data File : BP013799.D
 Acq On : 08 Feb 2023 16:22
 Operator : CG/JU
 Sample : 01422-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B69

Quant Time: Feb 08 23:56:26 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 08 00:37:14 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.122	152	151223	20.000	ng/u1	0.00
20) Naphthalene-d8	10.952	136	672794	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.757	164	469389	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.510	188	1136705	20.000	ng/u1	0.00
79) Chrysene-d12	21.586	240	1104032	20.000	ng/u1	0.00
88) Perylene-d12	24.151	264	989093	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.470	96	16595	4.548	ng/uL	0.00
4) Pyridine-d5	3.905	84	99091	9.161	ng/u1	0.00
7) Phenol-d5	7.269	99	85793	6.367	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.440	67	236033	29.895	ng/u1	0.00
11) 2-Chlorophenol-d4	7.646	132	237654	23.961	ng/u1	0.00
15) 4-Methylphenol-d8	8.828	113	178916	16.246	ng/u1	0.00
21) Nitrobenzene-d5	9.293	128	155078	33.128	ng/u1	0.00
24) 2-Nitrophenol-d4	10.022	143	169954	31.445	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.563	165	330134	29.973	ng/u1	0.00
31) 4-Chloroaniline-d4	11.081	131	387731	24.835	ng/u1	0.00
46) Dimethylphthalate-d6	14.157	166	1275749	34.507	ng/u1	0.00
49) Acenaphthylene-d8	14.451	160	1350299	33.741	ng/u1	0.00
54) 4-Nitrophenol-d4	14.940	143	30475	4.627	ng/u1	0.00
60) Fluorene-d10	15.751	176	1113713	35.367	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	162795	23.344	ng/u1	0.00
73) Anthracene-d10	17.610	188	1862758	35.838	ng/u1	0.00
81) Pyrene-d10	19.828	212	2338868	37.357	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.980	264	1859606	37.522	ng/u1	0.00
Target Compounds						
78) Di-n-butylphthalate	18.439	149	417689	6.460	ng/u1	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013799.D
Acq On : 08 Feb 2023 16:22
Operator : CG/JU
Sample : 01422-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B69

Quant Time: Feb 08 23:56:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 08 00:37:14 2023
Response via : Initial Calibration

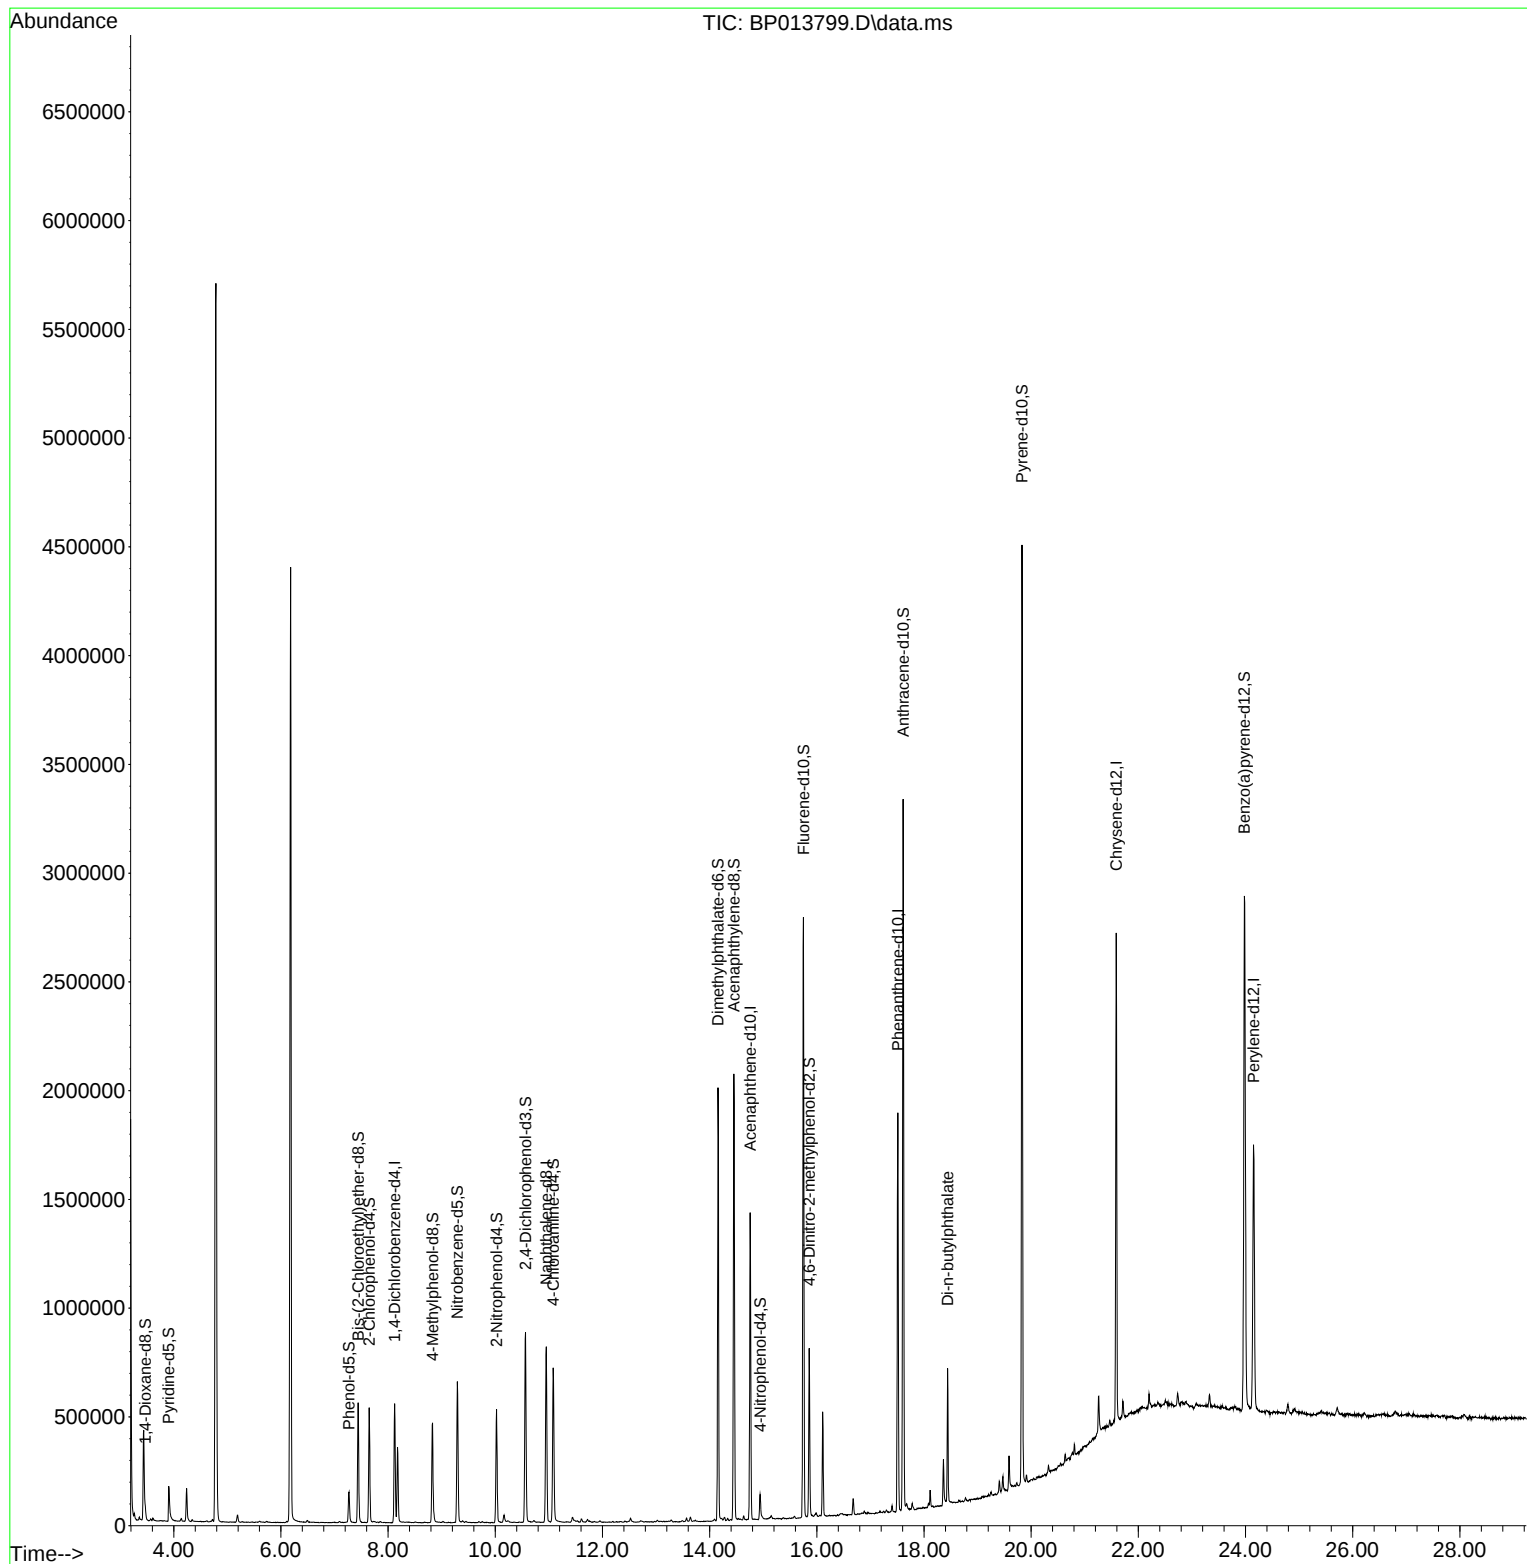

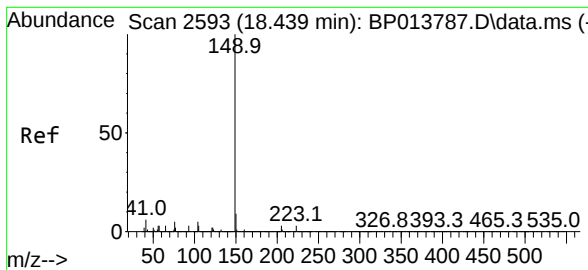

#78

Di-n-butylphthalate

Concen: 6.460 ng/ul

RT: 18.439 min Scan# 21

Delta R.T. -0.006 min

Lab File: BP013799.D


Acq: 08 Feb 2023 16:22

Instrument :

BNA_P

ClientSampleId :

C0B69

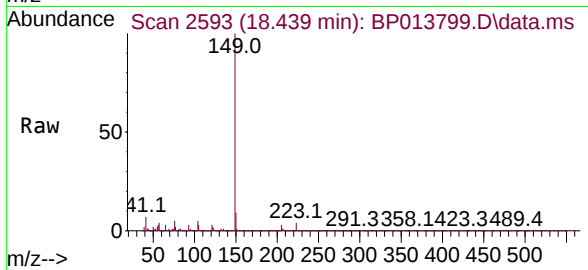

Tgt Ion:149 Resp: 417689

Ion Ratio Lower Upper

149 100

150 9.1 7.1 10.7

104 4.7 4.1 6.1

