

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
 Data File : BP013788.D
 Acq On : 08 Feb 2023 09:57
 Operator : CG/JU
 Sample : PB150698BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK698

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013788.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.469	44	48	54	rVB	41098	54666	1.02%	0.108%
2	3.899	118	121	140	rBV	511185	817161	15.24%	1.612%
3	4.240	174	179	187	rVB	10880	18515	0.35%	0.037%
4	7.269	684	694	708	rBV	619443	1035851	19.32%	2.043%
5	7.440	716	723	738	rVB	545683	847467	15.81%	1.672%
6	7.645	751	758	767	rBV	642080	1038902	19.38%	2.049%
7	8.122	831	839	852	rBV	596551	952491	17.77%	1.879%
8	8.822	951	958	975	rBV	787471	1340346	25.00%	2.644%
9	9.292	1028	1038	1050	rBV	589137	992891	18.52%	1.959%
10	10.022	1154	1162	1177	rBV	520191	856655	15.98%	1.690%
11	10.563	1246	1254	1269	rBV	809074	1387326	25.88%	2.737%
12	10.951	1312	1320	1334	rBV	875512	1484526	27.69%	2.929%
13	11.081	1334	1342	1359	rBV	824619	1442932	26.91%	2.846%
14	12.528	1581	1588	1595	rBV3	12838	25522	0.48%	0.050%
15	13.639	1772	1777	1783	rBV5	4518	6248	0.12%	0.012%
16	14.157	1857	1865	1879	rBV	1784712	2480377	46.27%	4.893%
17	14.457	1908	1916	1932	rBV	1816336	2781689	51.89%	5.487%
18	14.757	1959	1967	1977	rBV	1494408	2269844	42.34%	4.478%
19	14.939	1991	1998	2019	rBV	699632	1070747	19.97%	2.112%
20	15.751	2128	2136	2148	rBV	2559190	3620518	67.53%	7.142%
21	15.857	2148	2154	2165	rBV	735947	1034295	19.29%	2.040%
22	15.986	2172	2176	2183	rVB4	11718	20440	0.38%	0.040%
23	17.186	2375	2380	2383	rBV7	3804	6160	0.11%	0.012%
24	17.298	2395	2399	2406	rBV4	4007	7057	0.13%	0.014%
25	17.510	2429	2435	2445	rBV	1991972	2968410	55.37%	5.856%
26	17.610	2445	2452	2471	rVV	2931217	4172716	77.83%	8.232%
27	18.363	2577	2580	2586	rBV7	8804	16406	0.31%	0.032%
28	19.404	2753	2757	2762	rBV2	38378	53855	1.00%	0.106%
29	19.474	2765	2769	2773	rVB	37200	51871	0.97%	0.102%
30	19.827	2823	2829	2838	rBV	4007418	5321265	99.26%	10.497%
31	21.586	3123	3128	3137	rBV	2647252	3609664	67.33%	7.121%
32	23.986	3528	3536	3551	rVB2	2507326	5361123	100.00%	10.576%
33	24.150	3557	3564	3576	rVB2	1627447	3543513	66.10%	6.990%




Sum of corrected areas: 50691449

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013788.D
Acq On : 08 Feb 2023 09:57
Operator : CG/JU
Sample : PB150698BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK698

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

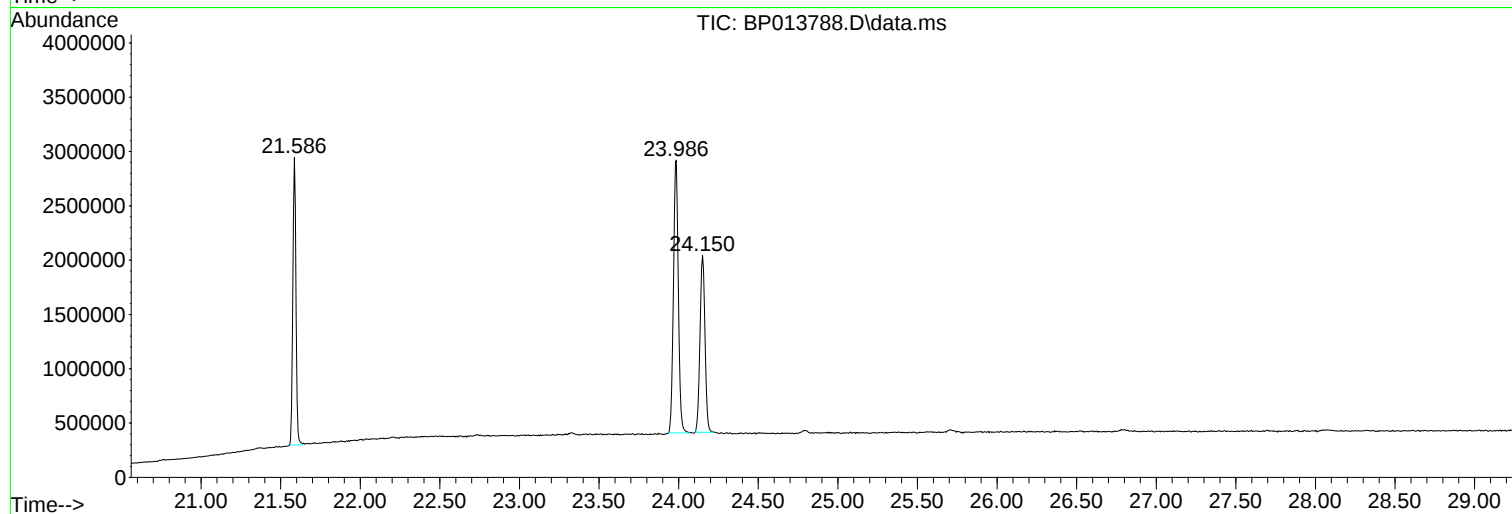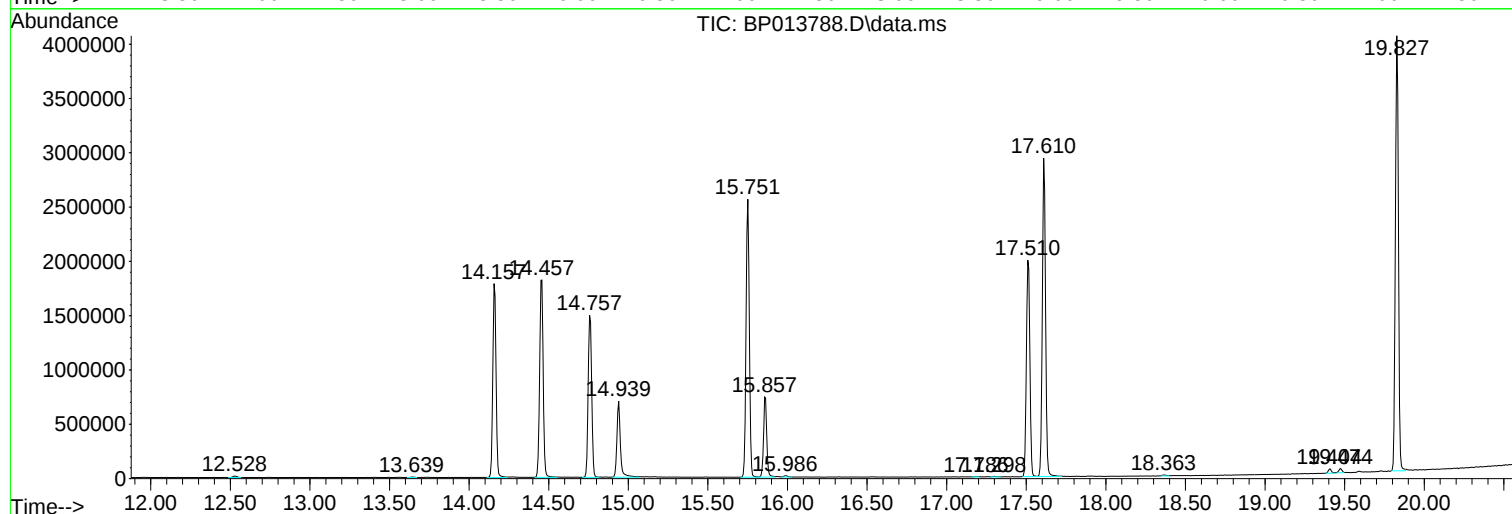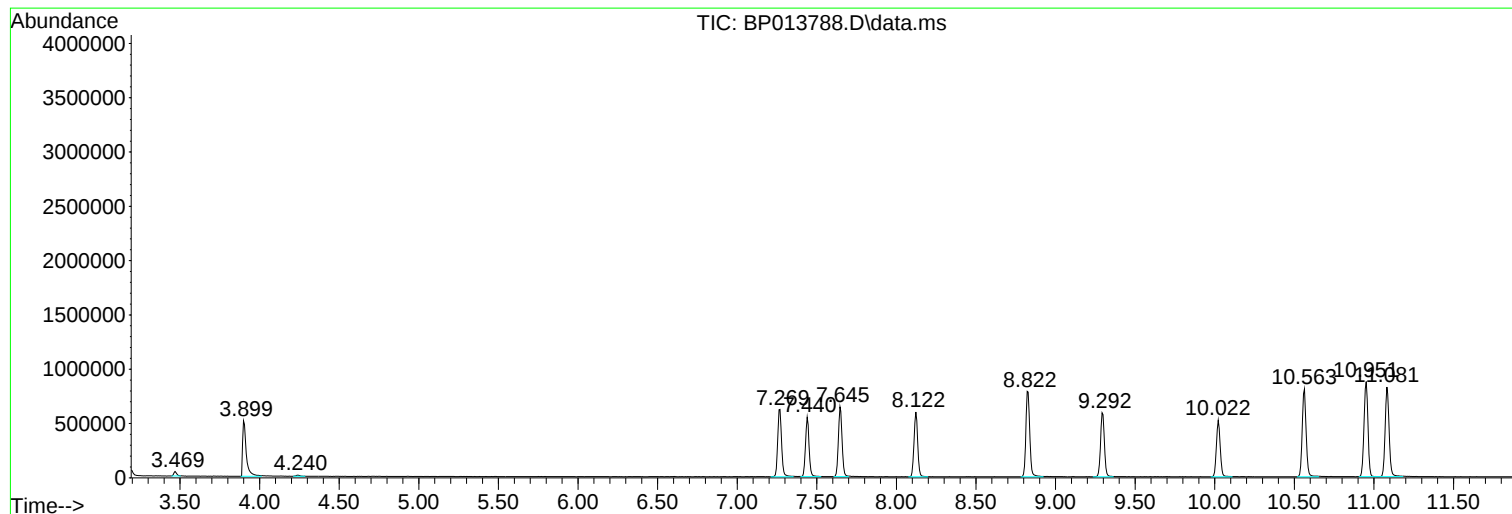

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013788.D
Acq On : 08 Feb 2023 09:57
Operator : CG/JU
Sample : PB150698BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK698

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013788.D
Acq On : 08 Feb 2023 09:57
Operator : CG/JU
Sample : PB150698BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK698

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc