

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
 Data File : BP013790.D
 Acq On : 08 Feb 2023 11:07
 Operator : CG/JU
 Sample : 01381-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44M8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013790.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.469	44	48	58	rVB	28737	41322	0.64%	0.092%
2	3.828	106	109	113	rVB3	11569	14328	0.22%	0.032%
3	3.911	120	123	144	rBV	115412	200653	3.10%	0.446%
4	4.140	158	162	168	rVB2	12546	19664	0.30%	0.044%
5	4.240	174	179	185	rBV	11170	16830	0.26%	0.037%
6	4.699	251	257	263	rBV2	9239	22915	0.35%	0.051%
7	5.399	371	376	385	rVB	25108	43731	0.67%	0.097%
8	5.569	403	405	406	rBV	10699	9384	0.14%	0.021%
9	6.158	500	505	517	rVB9	4145	10861	0.17%	0.024%
10	7.240	683	689	690	rBV5	6068	9254	0.14%	0.021%
11	7.275	690	695	708	rVV2	13375	48083	0.74%	0.107%
12	7.440	713	723	737	rVB	462107	797341	12.30%	1.772%
13	7.652	754	759	769	rBV	35061	77795	1.20%	0.173%
14	8.122	832	839	847	rBV	548831	916199	14.14%	2.036%
15	8.481	895	900	908	rVB2	17649	30187	0.47%	0.067%
16	8.840	949	961	979	rBV3	50307	187528	2.89%	0.417%
17	9.028	986	993	1003	rVB10	7499	21449	0.33%	0.048%
18	9.299	1031	1039	1054	rBV	393945	666022	10.28%	1.480%
19	9.699	1102	1107	1113	rBV5	7829	16415	0.25%	0.036%
20	9.752	1113	1116	1120	rVV4	10304	17519	0.27%	0.039%
21	9.793	1120	1123	1128	rVB6	6094	9298	0.14%	0.021%
22	10.034	1157	1164	1172	rBV6	5908	14096	0.22%	0.031%
23	10.210	1188	1194	1201	rBV5	10886	21902	0.34%	0.049%
24	10.569	1246	1255	1264	rBV2	41091	97395	1.50%	0.216%
25	10.810	1291	1296	1300	rBV7	4041	7870	0.12%	0.017%
26	10.951	1311	1320	1328	rBV	839256	1407864	21.72%	3.129%
27	11.081	1335	1342	1358	rBV	685949	1235117	19.06%	2.745%
28	11.616	1425	1433	1437	rBV2	9842	18357	0.28%	0.041%
29	11.898	1475	1481	1482	rBV5	5383	8861	0.14%	0.020%
30	12.087	1509	1513	1518	rBV7	5143	10396	0.16%	0.023%
31	12.193	1526	1531	1536	rBV3	13704	25345	0.39%	0.056%
32	12.463	1572	1577	1583	rBV4	6793	13342	0.21%	0.030%
33	12.522	1583	1587	1593	rVB2	11141	18476	0.29%	0.041%
34	13.175	1693	1698	1701	rBV3	6454	11110	0.17%	0.025%
35	13.645	1775	1778	1782	rVB6	6054	7996	0.12%	0.018%
36	14.069	1844	1850	1856	rBV6	8290	15951	0.25%	0.035%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
 Data File : BP013790.D
 Acq On : 08 Feb 2023 11:07
 Operator : CG/JU
 Sample : 01381-04
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44M8

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Title : SVOA CALIBRATION

37	14.157	1859	1865	1878	rVV	1213173	1697698	26.20%	3.773%
38	14.287	1881	1887	1890	rVB7	4848	9166	0.14%	0.020%
39	14.457	1909	1916	1929	rBV2	1958166	2973709	45.89%	6.608%
40	14.639	1942	1947	1952	rVB8	4387	7193	0.11%	0.016%
41	14.757	1960	1967	1976	rBV	1437023	2197815	33.91%	4.884%
42	15.010	2005	2010	2019	rBV2	10641	22690	0.35%	0.050%
43	15.751	2124	2136	2150	rBV	2863329	4148162	64.01%	9.218%
44	15.857	2152	2154	2160	rVB7	4195	6758	0.10%	0.015%
45	15.992	2170	2177	2183	rBV5	13775	24848	0.38%	0.055%
46	16.116	2193	2198	2206	rVB2	11924	19428	0.30%	0.043%
47	16.316	2230	2232	2238	rVB7	4537	6856	0.11%	0.015%
48	17.192	2377	2381	2387	rVB9	6602	12067	0.19%	0.027%
49	17.251	2387	2391	2395	rBV7	6813	11123	0.17%	0.025%
50	17.298	2395	2399	2404	rVV5	8094	12108	0.19%	0.027%
51	17.510	2428	2435	2445	rBV	2012748	2915358	44.99%	6.479%
52	17.610	2446	2452	2462	rVV2	3267101	4755990	73.39%	10.569%
53	18.363	2577	2580	2583	rBV5	8704	12427	0.19%	0.028%
54	19.404	2753	2757	2763	rBV2	56347	82806	1.28%	0.184%
55	19.475	2765	2769	2772	rBV2	43881	58258	0.90%	0.129%
56	19.827	2823	2829	2841	rBV	4584783	6276688	96.85%	13.948%
57	21.586	3123	3128	3139	rBV	2629176	3619045	55.84%	8.042%
58	23.986	3528	3536	3553	rVB2	3144340	6480551	100.00%	14.401%
59	24.151	3557	3564	3578	rVB2	1649721	3558284	54.91%	7.907%




Sum of corrected areas: 44999884

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013790.D
Acq On : 08 Feb 2023 11:07
Operator : CG/JU
Sample : 01381-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44M8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

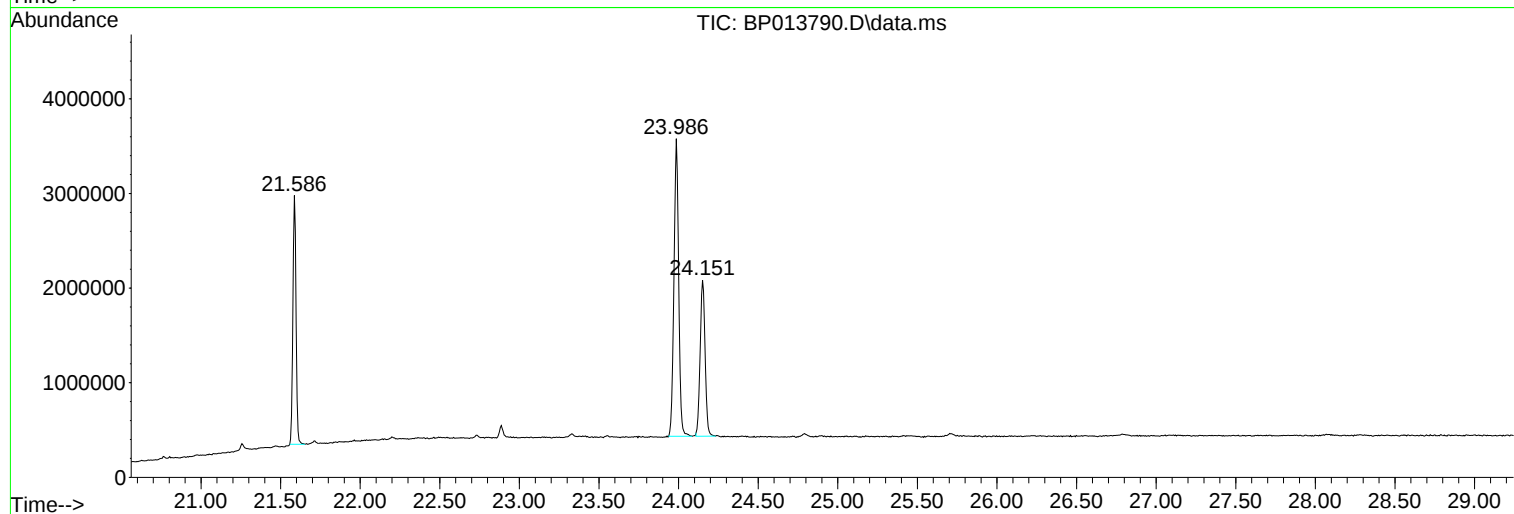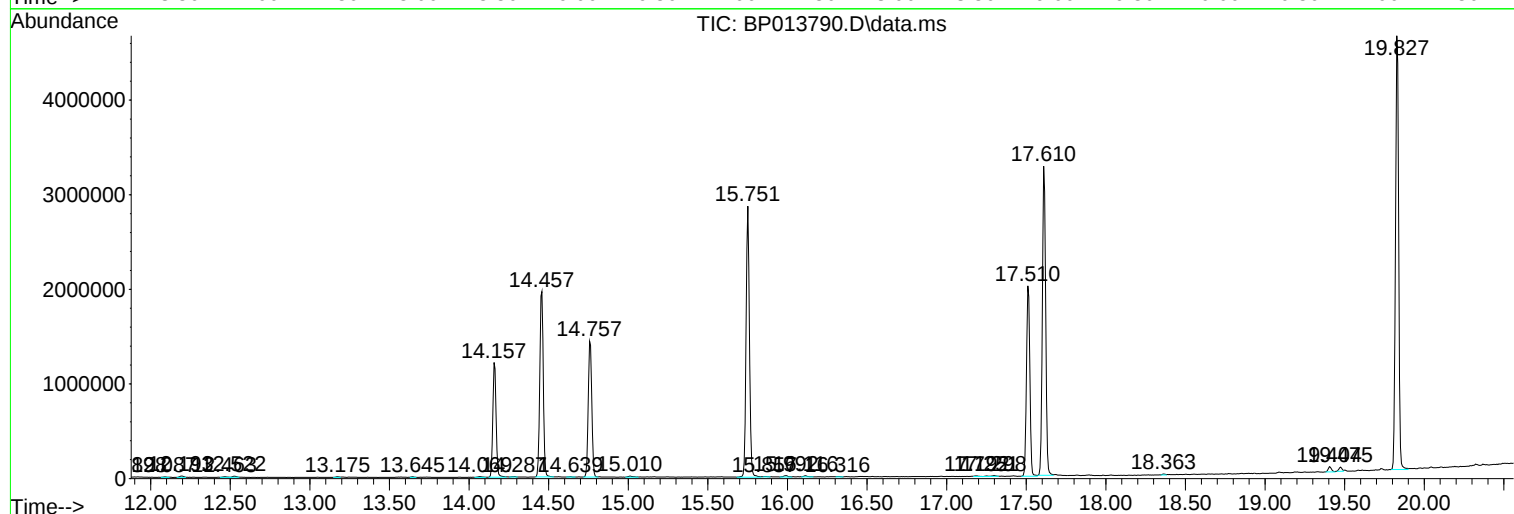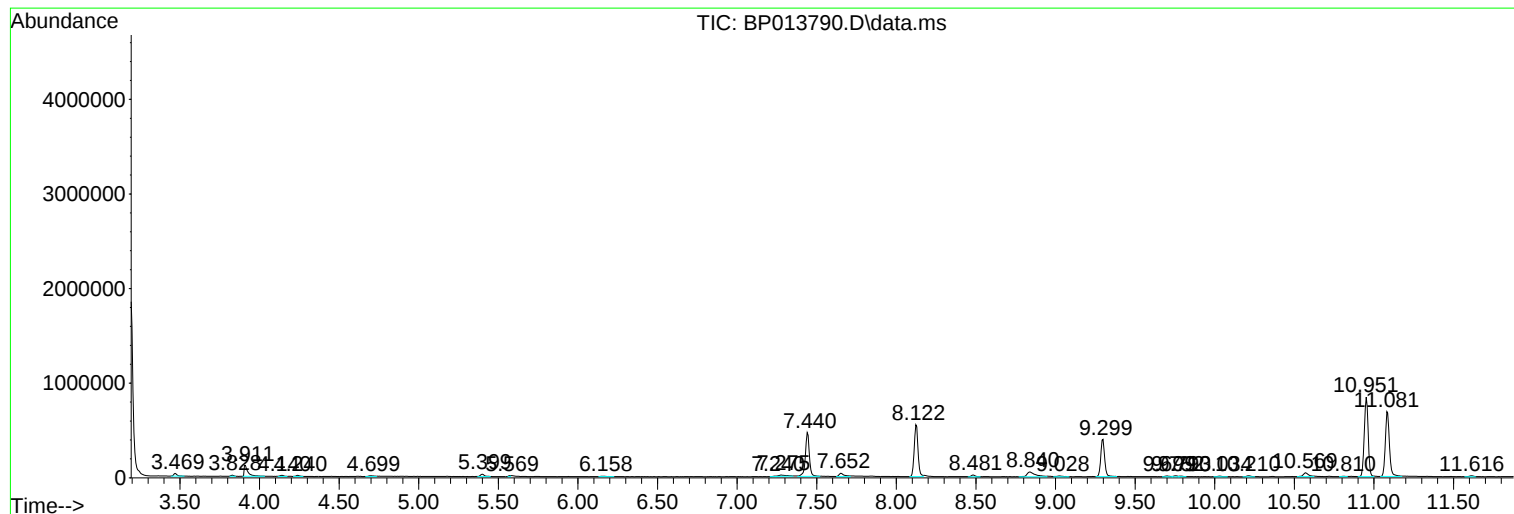

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013790.D
Acq On : 08 Feb 2023 11:07
Operator : CG/JU
Sample : 01381-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44M8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013790.D
Acq On : 08 Feb 2023 11:07
Operator : CG/JU
Sample : 01381-04
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44M8

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc