

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
 Data File : BP013792.D
 Acq On : 08 Feb 2023 12:22
 Operator : CG/JU
 Sample : 01381-10DL2 3000X
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44K7DL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013792.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.440	38	43	53	rVB	30148	50352	1.54%	0.353%
2	4.240	176	179	185	rVB2	8062	11152	0.34%	0.078%
3	5.399	368	376	388	rBV	123370	189842	5.80%	1.329%
4	8.016	816	821	829	rVB3	6911	12289	0.38%	0.086%
5	8.122	832	839	859	rVV	468596	853401	26.06%	5.975%
6	8.481	893	900	910	rBV	165393	279939	8.55%	1.960%
7	9.340	1038	1046	1060	rBV	466202	806852	24.63%	5.649%
8	10.810	1291	1296	1300	rBV8	2032	3324	0.10%	0.023%
9	10.951	1310	1320	1335	rBV	678677	1186316	36.22%	8.306%
10	12.187	1526	1530	1536	rBV6	2229	4629	0.14%	0.032%
11	14.151	1860	1864	1871	rBV9	2572	6449	0.20%	0.045%
12	14.763	1960	1968	1981	rBV	1189500	1848790	56.45%	12.945%
13	14.851	1981	1983	1993	rVB10	4391	10472	0.32%	0.073%
14	15.710	2123	2129	2133	rBV9	1661	3498	0.11%	0.024%
15	17.310	2397	2401	2405	rBV4	2644	3883	0.12%	0.027%
16	17.516	2429	2436	2450	rBV	1707072	2514268	76.76%	17.605%
17	18.363	2577	2580	2583	rBV5	6475	8552	0.26%	0.060%
18	21.586	3123	3128	3141	rBV	2306256	3275370	100.00%	22.934%
19	24.151	3557	3564	3576	rVB2	1486476	3212522	98.08%	22.494%




Sum of corrected areas: 14281900

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013792.D
Acq On : 08 Feb 2023 12:22
Operator : CG/JU
Sample : 01381-10DL2 3000X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44K7DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

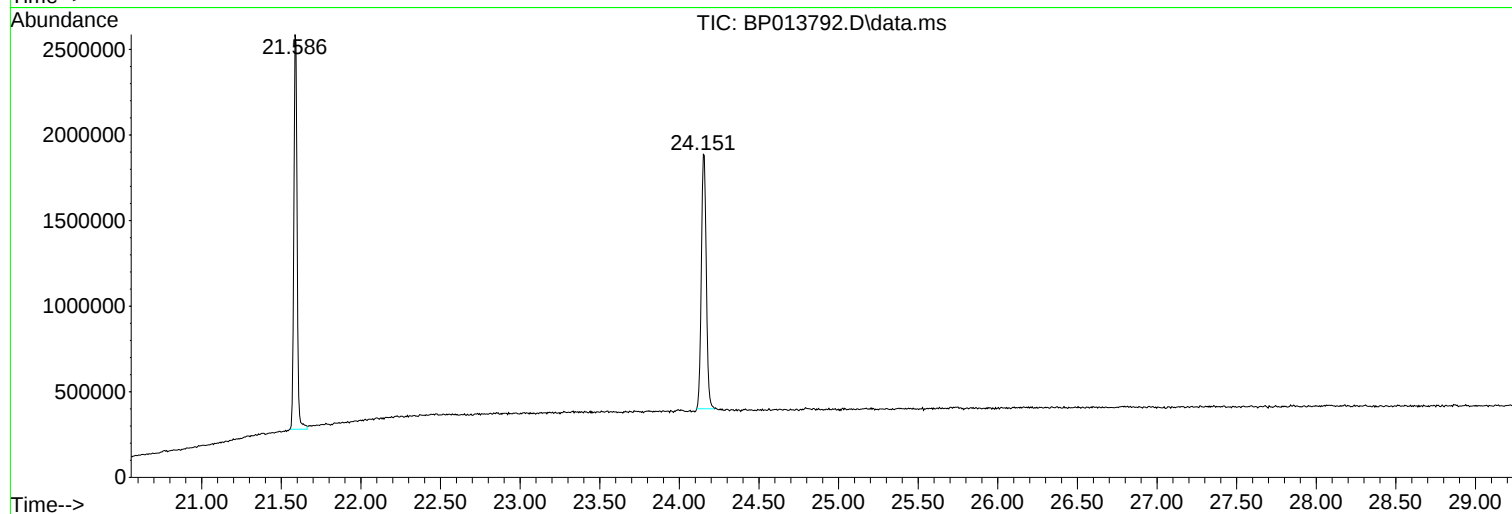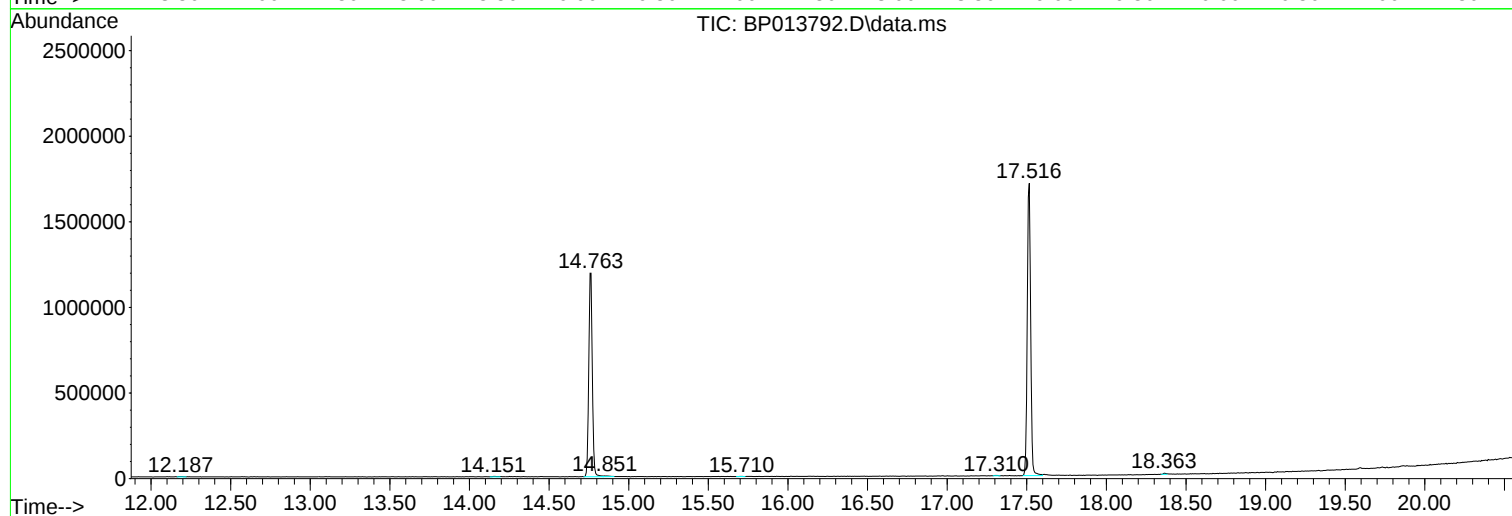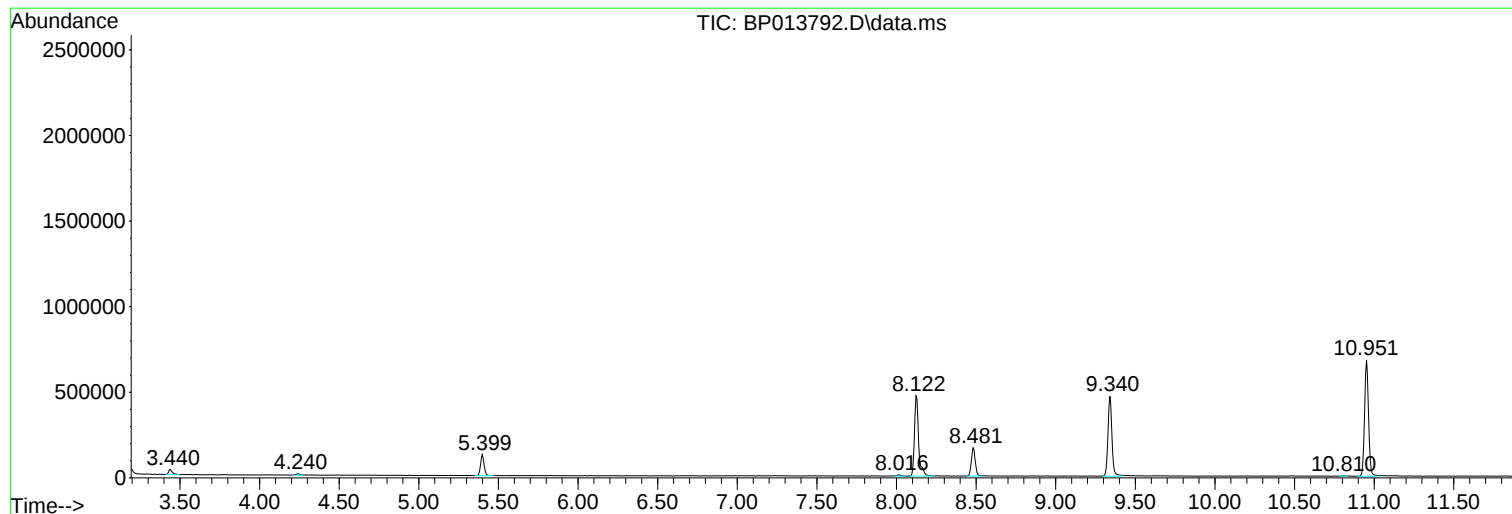

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013792.D
Acq On : 08 Feb 2023 12:22
Operator : CG/JU
Sample : 01381-10DL2 3000X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44K7DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013792.D
Acq On : 08 Feb 2023 12:22
Operator : CG/JU
Sample : 01381-10DL2 3000X
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44K7DL2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc