

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
 Data File : BP013797.D
 Acq On : 08 Feb 2023 15:14
 Operator : CG/JU
 Sample : 01422-04
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B63

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013797.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.469	43	48	56	rVB	31217	45888	0.73%	0.095%
2	3.911	120	123	138	rBV	88417	155300	2.47%	0.322%
3	4.140	157	162	166	rBV2	10611	15801	0.25%	0.033%
4	4.240	175	179	184	rVB	11132	18089	0.29%	0.038%
5	4.340	192	196	203	rVB8	7793	12681	0.20%	0.026%
6	5.187	335	340	348	rVB2	28351	48991	0.78%	0.102%
7	6.146	497	503	509	rBV10	3985	7191	0.11%	0.015%
8	6.493	557	562	568	rVB4	7033	13230	0.21%	0.027%
9	7.269	688	694	704	rVB	111401	183653	2.92%	0.381%
10	7.440	715	723	735	rBV	499890	788618	12.53%	1.638%
11	7.646	751	758	768	rBV	460638	758176	12.04%	1.574%
12	8.122	831	839	850	rBV	581420	933166	14.82%	1.938%
13	8.828	950	959	976	rBV	380722	652866	10.37%	1.356%
14	9.293	1031	1038	1051	rBV	556495	940651	14.94%	1.953%
15	9.446	1060	1064	1069	rVB3	10588	15832	0.25%	0.033%
16	10.022	1154	1162	1172	rBV	403573	665115	10.57%	1.381%
17	10.563	1247	1254	1268	rBV	708520	1208904	19.21%	2.510%
18	10.951	1312	1320	1333	rBV	827680	1417280	22.52%	2.943%
19	11.081	1334	1342	1367	rVV	674131	1176857	18.70%	2.444%
20	11.722	1447	1451	1460	rBV8	6377	13721	0.22%	0.028%
21	12.528	1582	1588	1593	rBV2	14707	24637	0.39%	0.051%
22	13.645	1773	1778	1784	rBV2	10849	16900	0.27%	0.035%
23	14.157	1859	1865	1877	rBV	1712865	2377631	37.77%	4.937%
24	14.269	1881	1884	1890	rVB8	3675	7152	0.11%	0.015%
25	14.451	1908	1915	1931	rBV	1822117	2669730	42.41%	5.544%
26	14.757	1959	1967	1977	rBV	1510431	2185352	34.72%	4.538%
27	14.939	1992	1998	2013	rBV	67439	148543	2.36%	0.308%
28	15.163	2031	2036	2044	rVB10	7583	16748	0.27%	0.035%
29	15.751	2126	2136	2148	rBV	2500287	3626566	57.61%	7.530%
30	15.857	2148	2154	2166	rVV	391467	565917	8.99%	1.175%
31	15.992	2172	2177	2182	rVB4	12004	18769	0.30%	0.039%
32	17.186	2376	2380	2384	rVB7	5816	8179	0.13%	0.017%
33	17.510	2429	2435	2445	rBV	1998955	2854570	45.35%	5.927%
34	17.610	2445	2452	2465	rBV2	3216206	4708654	74.80%	9.777%
35	17.786	2478	2482	2483	rBV3	4646	6561	0.10%	0.014%
36	17.892	2493	2500	2502	rBV6	5181	10194	0.16%	0.021%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013797.D
Acq On : 08 Feb 2023 15:14
Operator : CG/JU
Sample : 01422-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B63

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Title : SVOA CALIBRATION

37	18.363	2575	2580	2585	rBV2	25686	38275	0.61%	0.079%
38	19.404	2754	2757	2762	rBV	44677	54254	0.86%	0.113%
39	19.474	2765	2769	2773	rVV	45719	60050	0.95%	0.125%
40	19.586	2785	2788	2793	rBV6	15216	22650	0.36%	0.047%
41	19.827	2823	2829	2842	rBV	4483321	6141283	97.56%	12.752%
42	21.586	3123	3128	3139	rBV	2656507	3651388	58.01%	7.582%
43	23.986	3528	3536	3546	rBV2	2887908	6294605	100.00%	13.071%
44	24.151	3557	3564	3577	rVB2	1693630	3578168	56.84%	7.430%




Sum of corrected areas: 48158786

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013797.D
Acq On : 08 Feb 2023 15:14
Operator : CG/JU
Sample : 01422-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B63

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

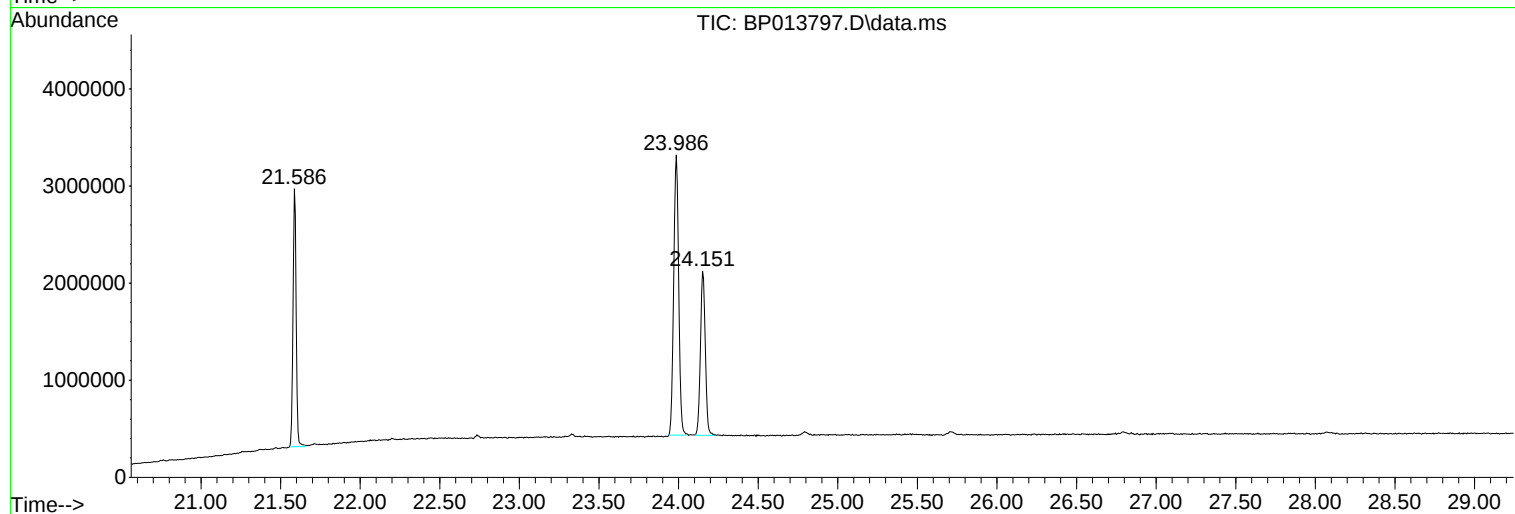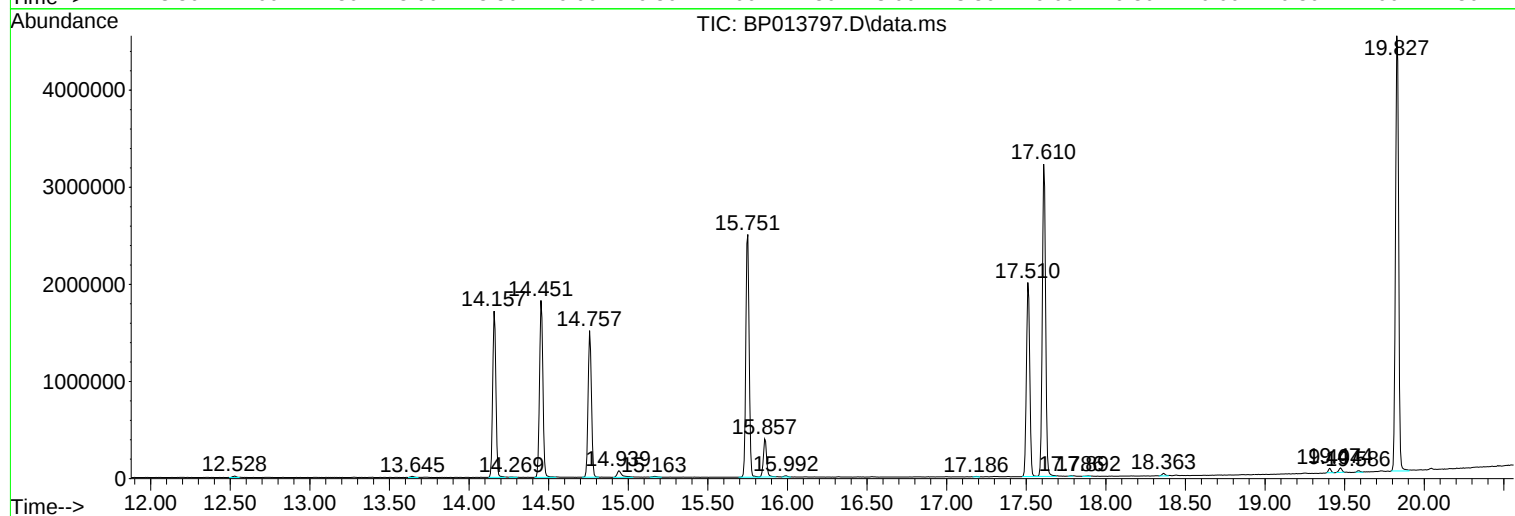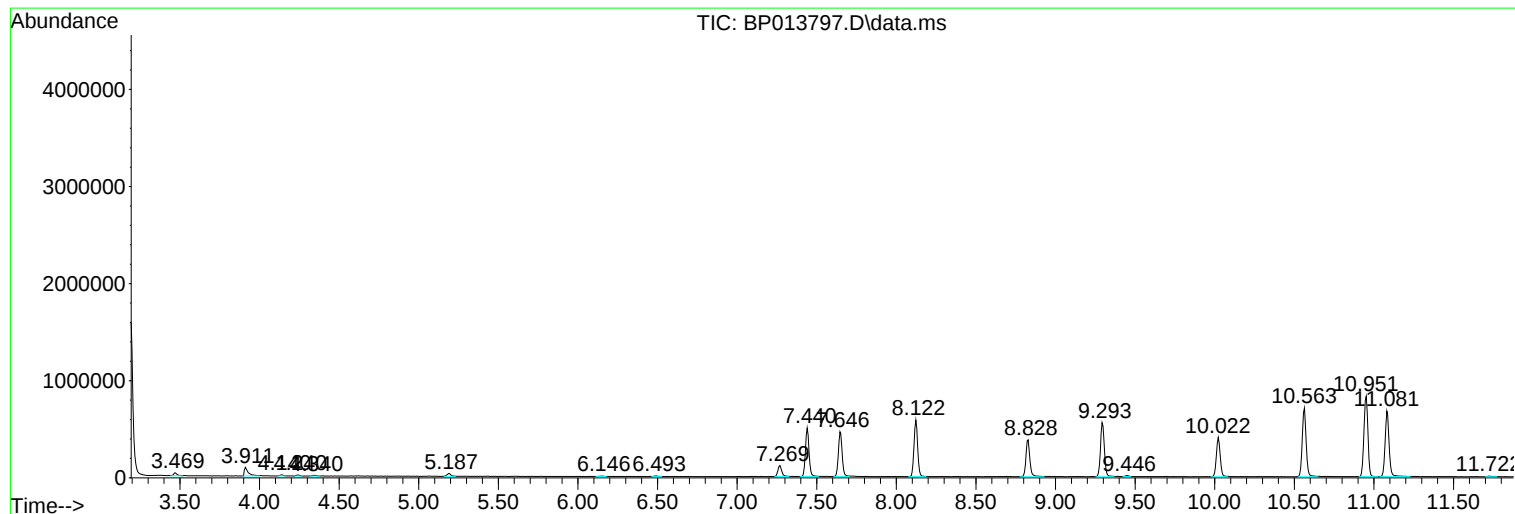

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013797.D
Acq On : 08 Feb 2023 15:14
Operator : CG/JU
Sample : 01422-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B63

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013797.D
Acq On : 08 Feb 2023 15:14
Operator : CG/JU
Sample : 01422-04
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B63

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc