

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
 Data File : BP013800.D
 Acq On : 08 Feb 2023 16:56
 Operator : CG/JU
 Sample : 01422-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013800.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.469	44	48	55	rVB	36062	50075	0.78%	0.098%
2	3.575	61	66	72	rBV4	6493	12943	0.20%	0.025%
3	3.905	119	122	137	rBV	158460	263376	4.10%	0.513%
4	4.140	157	162	167	rVB	13713	22867	0.36%	0.045%
5	4.240	174	179	184	rBV	12166	17144	0.27%	0.033%
6	4.346	192	197	202	rBV4	11339	15820	0.25%	0.031%
7	4.716	257	260	266	rVB6	4555	7047	0.11%	0.014%
8	5.187	333	340	347	rVB2	17801	35200	0.55%	0.069%
9	6.487	557	561	565	rBV4	8362	12842	0.20%	0.025%
10	7.269	681	694	708	rBV	137850	248102	3.86%	0.483%
11	7.440	715	723	739	rBV	600870	942462	14.66%	1.835%
12	7.646	751	758	768	rBV	540158	887634	13.81%	1.729%
13	8.122	832	839	851	rBV	617420	982746	15.29%	1.914%
14	8.828	949	959	973	rBV	447216	756862	11.78%	1.474%
15	9.022	988	992	999	rVB3	5567	10216	0.16%	0.020%
16	9.293	1030	1038	1052	rBV	719419	1176040	18.30%	2.290%
17	9.451	1057	1065	1069	rBV3	13496	21735	0.34%	0.042%
18	10.022	1153	1162	1171	rBV	556968	923139	14.36%	1.798%
19	10.563	1244	1254	1266	rBV	855573	1488324	23.16%	2.898%
20	10.951	1312	1320	1333	rVB	896066	1511798	23.52%	2.944%
21	11.081	1333	1342	1355	rBV	828161	1469729	22.87%	2.862%
22	12.528	1581	1588	1600	rVB2	16728	32556	0.51%	0.063%
23	13.639	1771	1777	1783	rBV4	15520	27694	0.43%	0.054%
24	14.157	1858	1865	1878	rBV	2015092	2860288	44.50%	5.570%
25	14.457	1908	1916	1928	rBV	2104733	3220580	50.11%	6.272%
26	14.757	1960	1967	1977	rBV	1522265	2276232	35.41%	4.433%
27	14.939	1991	1998	2013	rBV	100910	204703	3.18%	0.399%
28	15.163	2032	2036	2043	rVB7	8957	14942	0.23%	0.029%
29	15.428	2074	2081	2087	rBV4	9752	15607	0.24%	0.030%
30	15.751	2129	2136	2148	rBV	2968928	4294300	66.81%	8.363%
31	15.857	2148	2154	2166	rVV	608531	845360	13.15%	1.646%
32	15.986	2172	2176	2185	rVB2	14533	21896	0.34%	0.043%
33	17.304	2396	2400	2404	rBV5	5341	8760	0.14%	0.017%
34	17.510	2428	2435	2445	rBV	2045658	2980843	46.38%	5.805%
35	17.610	2445	2452	2462	rVV	3512134	5019357	78.09%	9.775%
36	17.692	2464	2466	2472	rVB5	16127	18972	0.30%	0.037%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
 Data File : BP013800.D
 Acq On : 08 Feb 2023 16:56
 Operator : CG/JU
 Sample : 01422-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0B73

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Title : SVOA CALIBRATION

37	17.880	2496	2498	2504	rBV5	4211	7185	0.11%	0.014%
38	18.151	2540	2544	2548	rVB7	5376	9302	0.14%	0.018%
39	18.363	2576	2580	2584	rBV5	15237	23356	0.36%	0.045%
40	19.233	2724	2728	2729	rBV4	10323	13883	0.22%	0.027%
41	19.404	2753	2757	2763	rBV2	49638	72672	1.13%	0.142%
42	19.474	2765	2769	2774	rVB	52525	70262	1.09%	0.137%
43	19.586	2786	2788	2791	rBV4	13392	14729	0.23%	0.029%
44	19.827	2823	2829	2842	rBV	4865453	6427547	100.00%	12.517%
45	21.586	3123	3128	3137	rBV	2636848	3488657	54.28%	6.794%
46	23.986	3528	3536	3545	rBV2	2520866	5486828	85.36%	10.685%
47	24.151	3557	3564	3577	rVB2	1384498	3036294	47.24%	5.913%




Sum of corrected areas: 51348906

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013800.D
Acq On : 08 Feb 2023 16:56
Operator : CG/JU
Sample : 01422-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B73

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

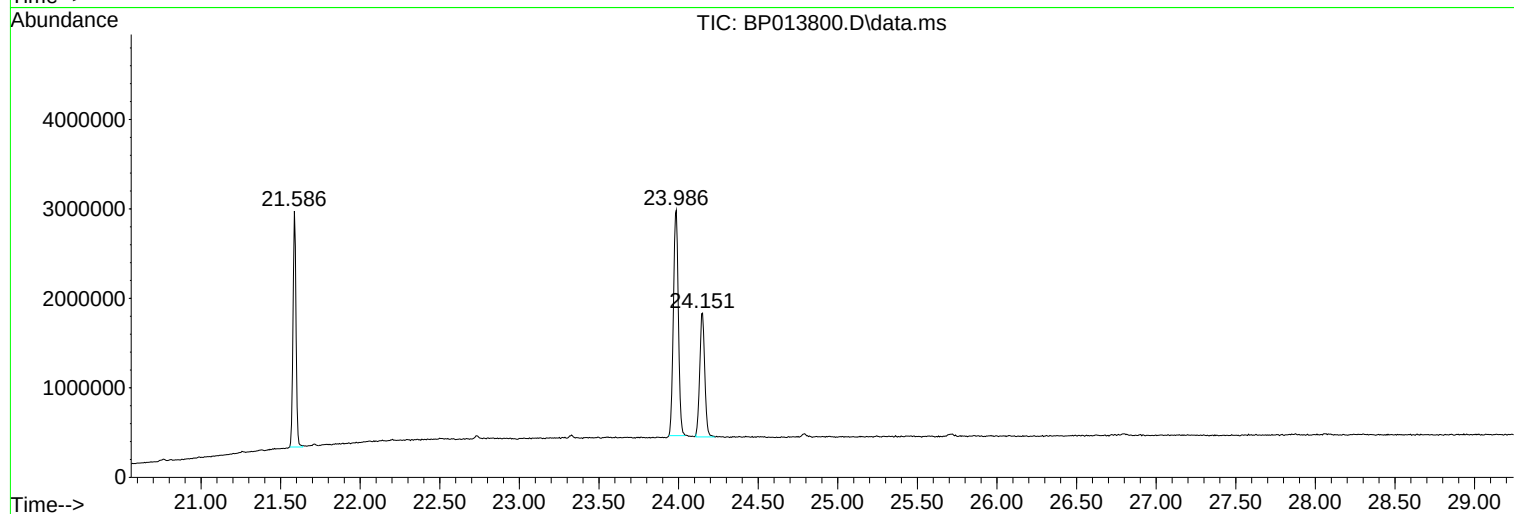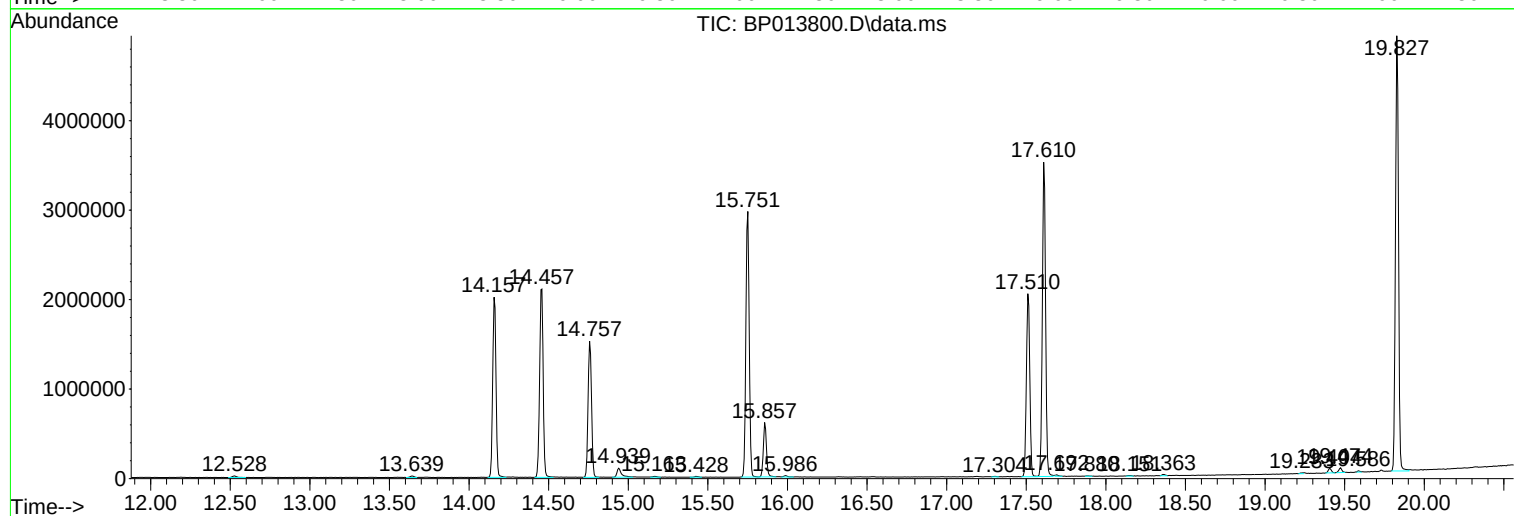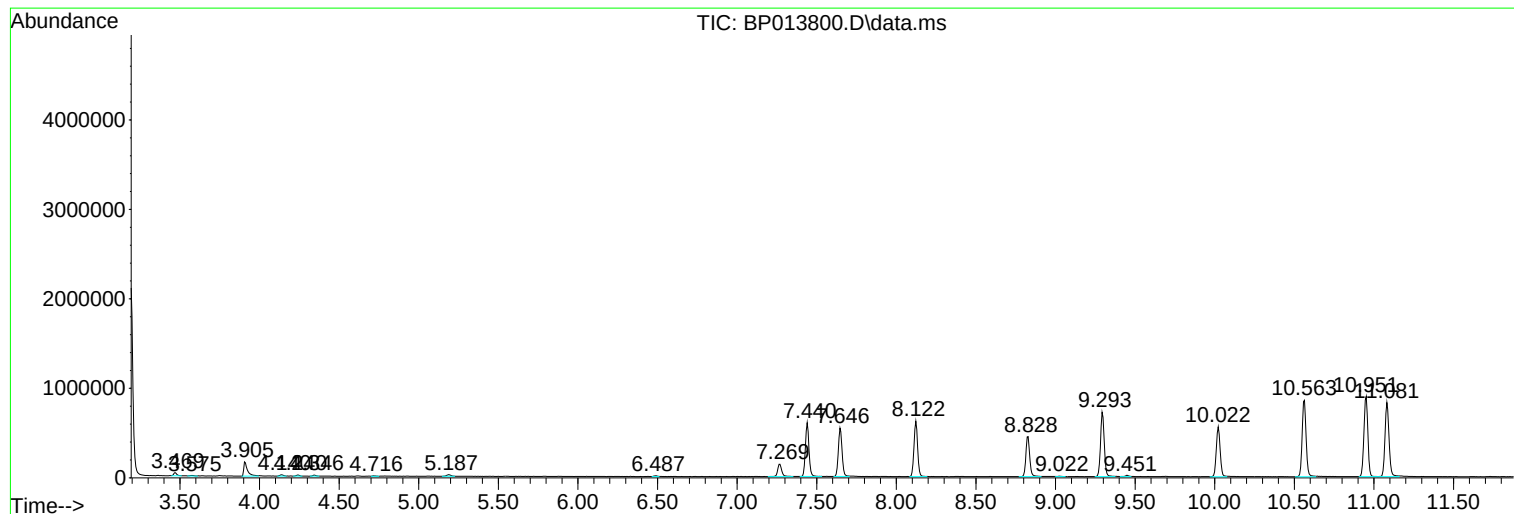

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013800.D
Acq On : 08 Feb 2023 16:56
Operator : CG/JU
Sample : 01422-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B73

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013800.D
Acq On : 08 Feb 2023 16:56
Operator : CG/JU
Sample : 01422-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0B73

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc