

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
 Data File : BP013803.D
 Acq On : 08 Feb 2023 18:40
 Operator : CG/JU
 Sample : PB150697BL
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK697

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013803.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.470	44	48	58	rVB	46531	63788	1.04%	0.111%
2	3.899	119	121	142	rBV	584146	927021	15.14%	1.613%
3	4.240	173	179	186	rBV	11486	15799	0.26%	0.027%
4	7.269	687	694	708	rBV	722631	1189352	19.42%	2.069%
5	7.440	717	723	735	rBV	615357	951967	15.55%	1.656%
6	7.646	751	758	774	rBV	745688	1201844	19.63%	2.091%
7	8.122	831	839	854	rVB	674669	1084217	17.71%	1.886%
8	8.828	951	959	975	rBV	958303	1626971	26.57%	2.831%
9	9.293	1028	1038	1050	rBV	735854	1228311	20.06%	2.137%
10	10.022	1152	1162	1178	rBV	635412	1062276	17.35%	1.848%
11	10.563	1246	1254	1270	rBV	971473	1725007	28.17%	3.001%
12	10.951	1311	1320	1329	rBV	987775	1690763	27.61%	2.942%
13	11.081	1335	1342	1360	rBV	1012998	1771868	28.94%	3.083%
14	12.522	1581	1587	1595	rBV	15992	33010	0.54%	0.057%
15	13.640	1769	1777	1783	rBV2	19986	33068	0.54%	0.058%
16	13.728	1789	1792	1801	rVB10	3165	6154	0.10%	0.011%
17	14.157	1857	1865	1877	rBV	2064381	2856180	46.64%	4.970%
18	14.451	1908	1915	1928	rBV	2128794	3236262	52.85%	5.631%
19	14.757	1959	1967	1980	rBV	1664912	2489513	40.66%	4.332%
20	14.939	1991	1998	2013	rBV	827277	1271718	20.77%	2.213%
21	15.163	2033	2036	2043	rVB9	4763	8827	0.14%	0.015%
22	15.751	2129	2136	2147	rBV	2808315	4200799	68.60%	7.309%
23	15.857	2148	2154	2168	rVV	696196	962845	15.72%	1.675%
24	15.986	2172	2176	2184	rVB	14923	24286	0.40%	0.042%
25	16.322	2228	2233	2237	rBV7	3269	6848	0.11%	0.012%
26	17.186	2376	2380	2384	rBV5	4236	7624	0.12%	0.013%
27	17.298	2396	2399	2405	rVB3	4371	7534	0.12%	0.013%
28	17.510	2428	2435	2445	rBV	2442367	3507318	57.28%	6.102%
29	17.610	2446	2452	2465	rVV2	3585268	5101978	83.32%	8.877%
30	18.363	2577	2580	2585	rBV6	7514	10122	0.17%	0.018%
31	18.439	2590	2593	2598	rBV	8504	12688	0.21%	0.022%
32	19.404	2753	2757	2762	rBV	53515	69547	1.14%	0.121%
33	19.475	2765	2769	2772	rVV	46023	58876	0.96%	0.102%
34	19.827	2823	2829	2840	rBV	4446526	6123497	100.00%	10.654%
35	21.586	3123	3128	3138	rBV	2856261	3889940	63.52%	6.768%
36	23.986	3528	3536	3548	rBV2	2576827	5499301	89.81%	9.568%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013803.D
Acq On : 08 Feb 2023 18:40
Operator : CG/JU
Sample : PB150697BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK697

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Title : SVOA CALIBRATION

37	24.151	3557	3564	3577	rVB2	1592538	3516517	57.43%	6.118%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 57473636

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013803.D
Acq On : 08 Feb 2023 18:40
Operator : CG/JU
Sample : PB150697BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK697

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

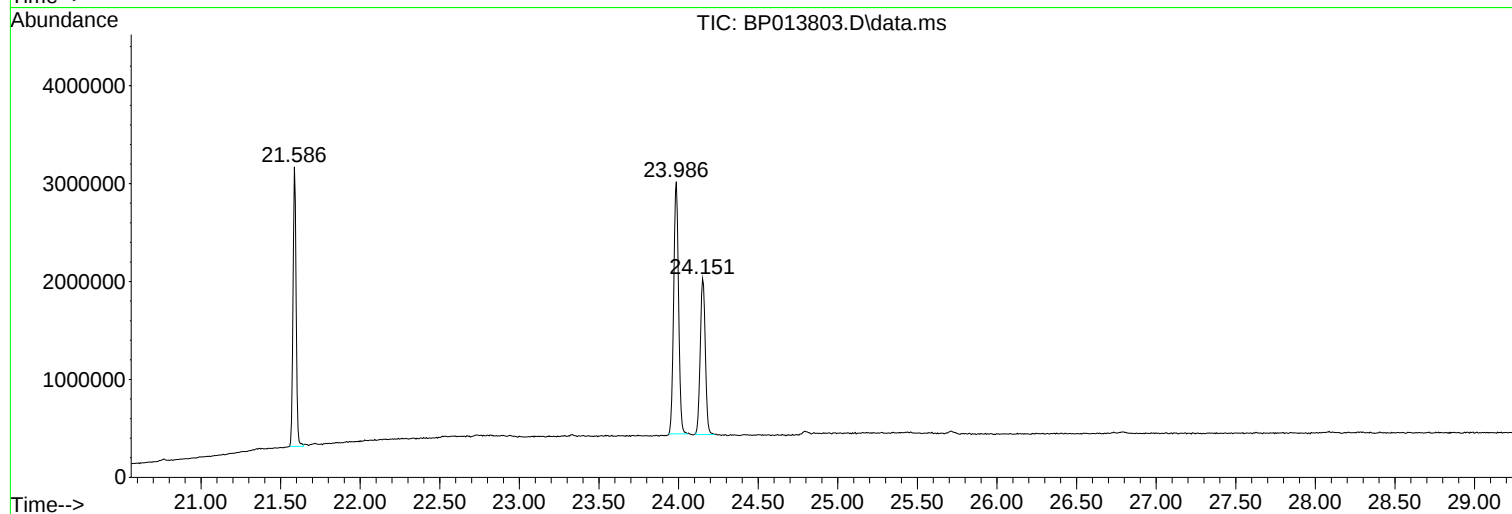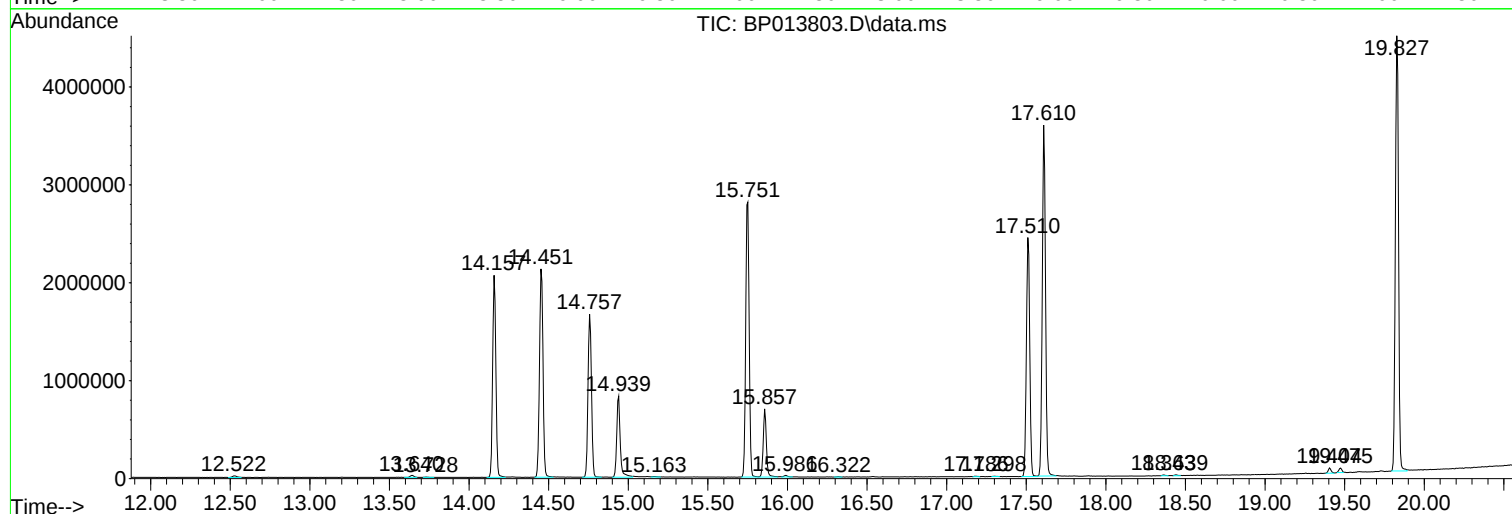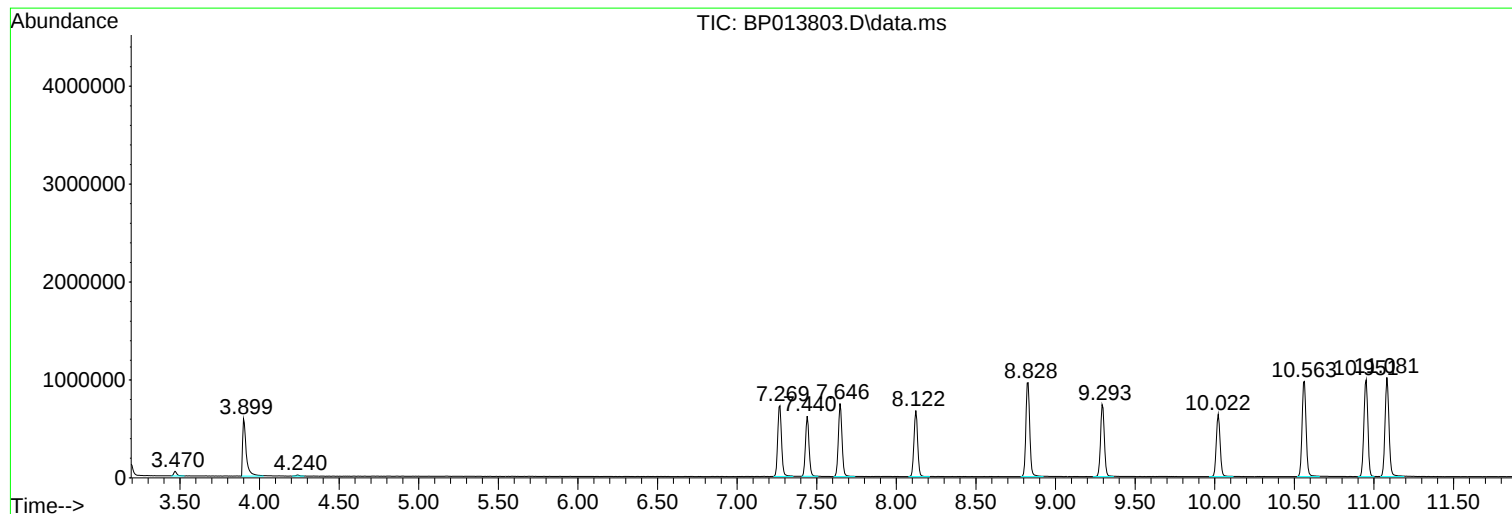

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013803.D
Acq On : 08 Feb 2023 18:40
Operator : CG/JU
Sample : PB150697BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK697

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020823\
Data File : BP013803.D
Acq On : 08 Feb 2023 18:40
Operator : CG/JU
Sample : PB150697BL
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK697

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc