

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020923\
 Data File : BP013808.D
 Acq On : 09 Feb 2023 10:26
 Operator : CG/JU
 Sample : 01497-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EW4X0

Quant Time: Feb 09 13:17:29 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Feb 08 00:37:14 2023
 Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.122	152	165516	20.000	ng/u1	0.00
20) Naphthalene-d8	10.946	136	739157	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.757	164	537021	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.510	188	1306064	20.000	ng/u1	0.00
79) Chrysene-d12	21.586	240	1382912	20.000	ng/u1	0.00
88) Perylene-d12	24.151	264	1389861	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.469	96	21822	5.465	ng/uL	0.00
4) Pyridine-d5	3.899	84	314118	26.532	ng/u1	0.00
7) Phenol-d5	7.263	99	423026	28.685	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.440	67	250076	28.938	ng/u1	0.00
11) 2-Chlorophenol-d4	7.646	132	313972	28.922	ng/u1	0.00
15) 4-Methylphenol-d8	8.822	113	352894	29.277	ng/u1	0.00
21) Nitrobenzene-d5	9.293	128	152687	29.689	ng/u1	0.00
24) 2-Nitrophenol-d4	10.022	143	183271	30.864	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.557	165	345978	28.591	ng/u1	0.00
31) 4-Chloroaniline-d4	11.081	131	499555	29.124	ng/u1	0.00
46) Dimethylphthalate-d6	14.157	166	1334543	31.552	ng/u1	0.00
49) Acenaphthylene-d8	14.451	160	1379580	30.131	ng/u1	0.00
54) 4-Nitrophenol-d4	14.939	143	194144	25.764	ng/u1	0.00
60) Fluorene-d10	15.745	176	1123998	31.198	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.857	200	165463	20.650	ng/u1	0.00
73) Anthracene-d10	17.610	188	1942002	32.518	ng/u1	0.00
81) Pyrene-d10	19.827	212	2491308	31.767	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.980	264	2358906	33.872	ng/u1	0.00
Target Compounds						
2) 1,4-Dioxane	3.505	88	13572	3.166	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020923\
Data File : BP013808.D
Acq On : 09 Feb 2023 10:26
Operator : CG/JU
Sample : 01497-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EW4X0

Quant Time: Feb 09 13:17:29 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Feb 08 00:37:14 2023
Response via : Initial Calibration

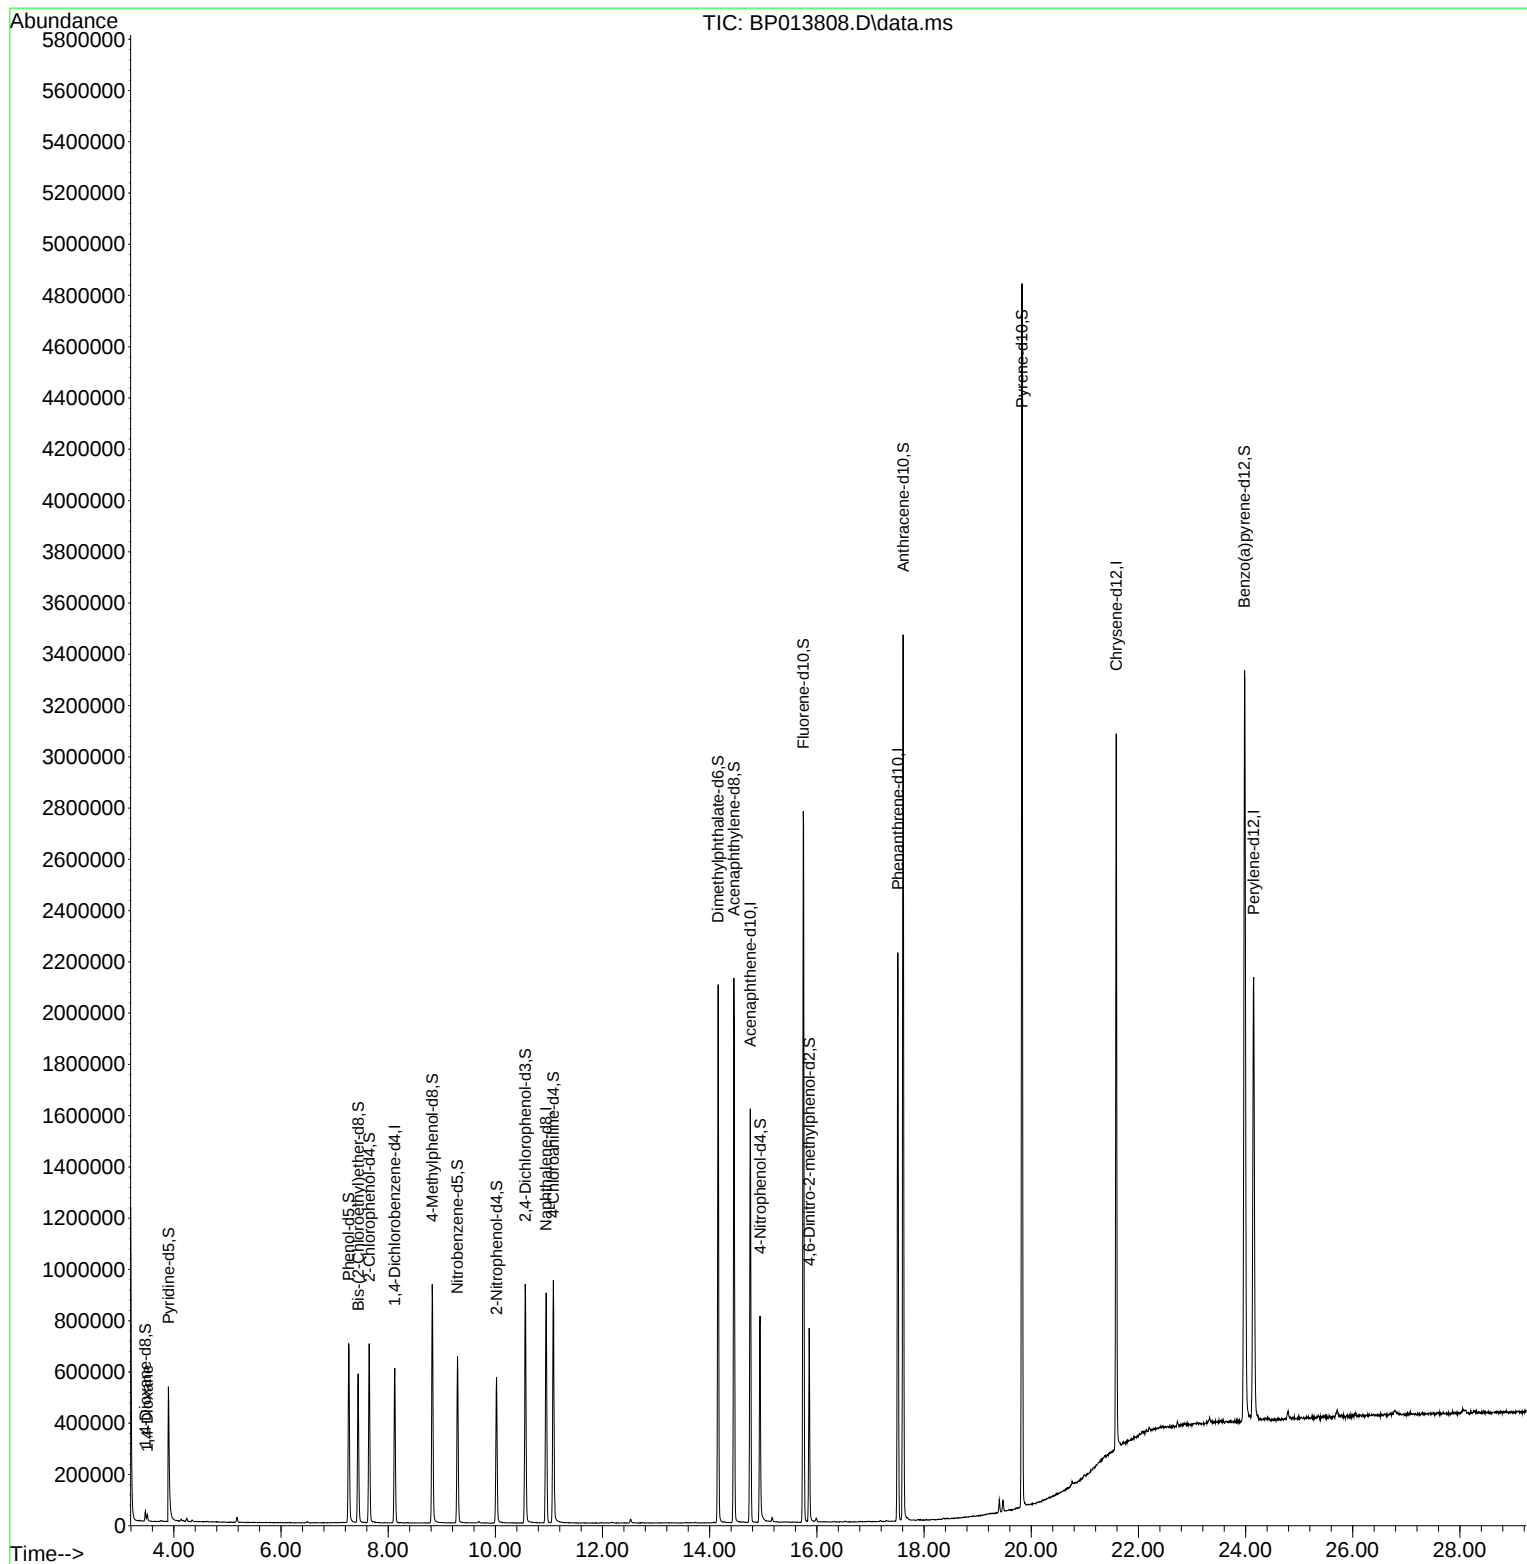

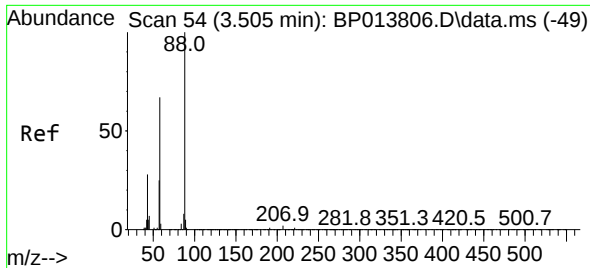

#2
 1,4-Dioxane
 Concen: 3.166 ng/uL
 RT: 3.505 min Scan# 54
 Delta R.T. -0.000 min
 Lab File: BP013808.D
 Acq: 09 Feb 2023 10:26

Instrument :
 BNA_P
 ClientSampleId :
 EW4X0

Tgt Ion:	88	Resp:	13572
Ion	Ratio	Lower	Upper
88	100		
43	25.1	20.1	30.1
58	68.7	53.0	79.6

