

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020923\
 Data File : BP013807.D
 Acq On : 09 Feb 2023 09:51
 Operator : CG/JU
 Sample : PB150744BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK744

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013807.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.470	43	48	58	rVB	35467	53642	1.01%	0.117%
2	3.899	118	121	136	rBV	433599	719943	13.59%	1.564%
3	4.234	175	178	184	rVB	10256	15012	0.28%	0.033%
4	7.263	685	693	710	rBV	561638	915774	17.29%	1.989%
5	7.440	717	723	738	rVB	469921	731747	13.82%	1.589%
6	7.646	750	758	772	rBV	567572	914694	17.27%	1.987%
7	8.122	831	839	855	rVB	518403	839479	15.85%	1.823%
8	8.822	951	958	975	rBV	703139	1170226	22.10%	2.542%
9	9.293	1029	1038	1049	rBV	514352	845325	15.96%	1.836%
10	10.022	1154	1162	1179	rBV	426249	730538	13.79%	1.587%
11	10.557	1246	1253	1271	rBV	709828	1216042	22.96%	2.641%
12	10.946	1312	1319	1329	rBV	780178	1302011	24.59%	2.828%
13	11.081	1335	1342	1357	rBV	720484	1254813	23.69%	2.725%
14	12.175	1522	1528	1534	rBV9	2332	5375	0.10%	0.012%
15	12.528	1581	1588	1593	rBV3	12261	22408	0.42%	0.049%
16	14.157	1856	1865	1879	rBV	1551874	2122517	40.08%	4.610%
17	14.451	1908	1915	1931	rBV	1590600	2404235	45.40%	5.222%
18	14.757	1960	1967	1977	rBV	1420801	2001760	37.80%	4.348%
19	14.940	1991	1998	2017	rBV	574973	935407	17.66%	2.032%
20	15.745	2124	2135	2148	rBV	2183331	3206230	60.54%	6.964%
21	15.857	2148	2154	2165	rVV	510697	698521	13.19%	1.517%
22	15.987	2172	2176	2182	rVB5	10580	17818	0.34%	0.039%
23	17.192	2374	2381	2383	rBV7	3474	5976	0.11%	0.013%
24	17.510	2428	2435	2445	rBV	1925796	2692771	50.85%	5.848%
25	17.610	2445	2452	2465	rVV2	2642450	3722010	70.28%	8.084%
26	18.363	2577	2580	2582	rBV4	4997	6725	0.13%	0.015%
27	19.404	2753	2757	2763	rBV3	35584	55824	1.05%	0.121%
28	19.475	2765	2769	2772	rBV	34678	46385	0.88%	0.101%
29	19.828	2823	2829	2841	rBV	3818813	4980434	94.04%	10.817%
30	21.586	3123	3128	3138	rBV2	2572713	3572461	67.46%	7.759%
31	23.980	3528	3535	3551	rVB2	2448853	5295944	100.00%	11.502%
32	24.151	3557	3564	3576	rVB	1684847	3540513	66.85%	7.690%




Sum of corrected areas: 46042560

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020923\
Data File : BP013807.D
Acq On : 09 Feb 2023 09:51
Operator : CG/JU
Sample : PB150744BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK744

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

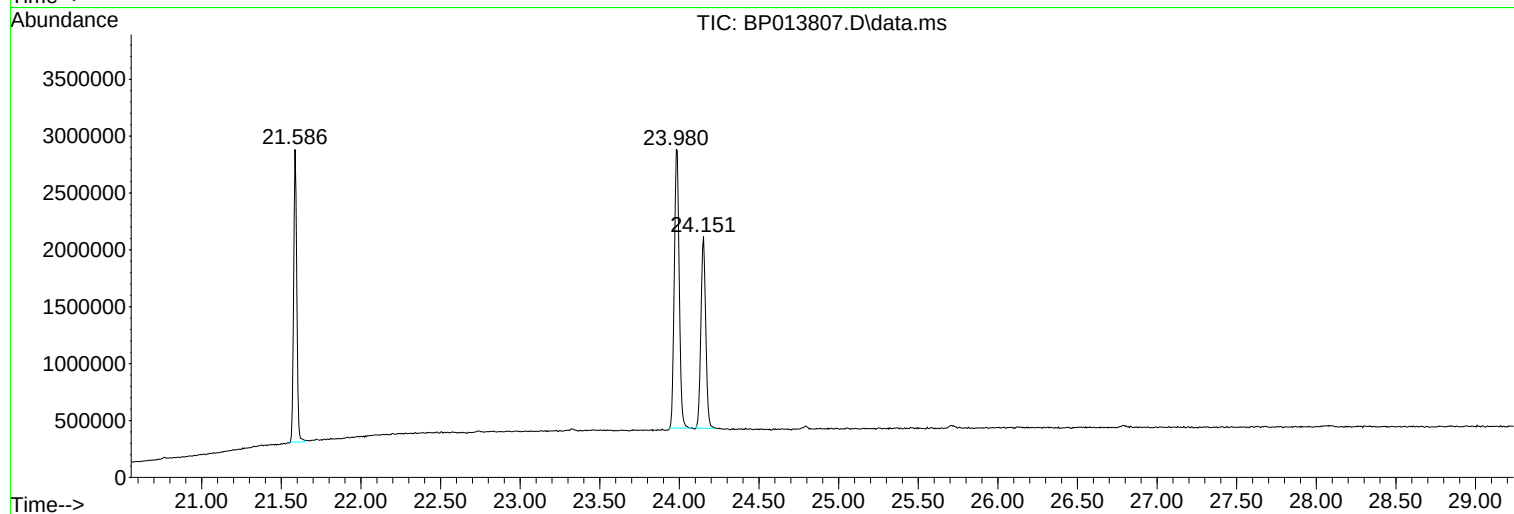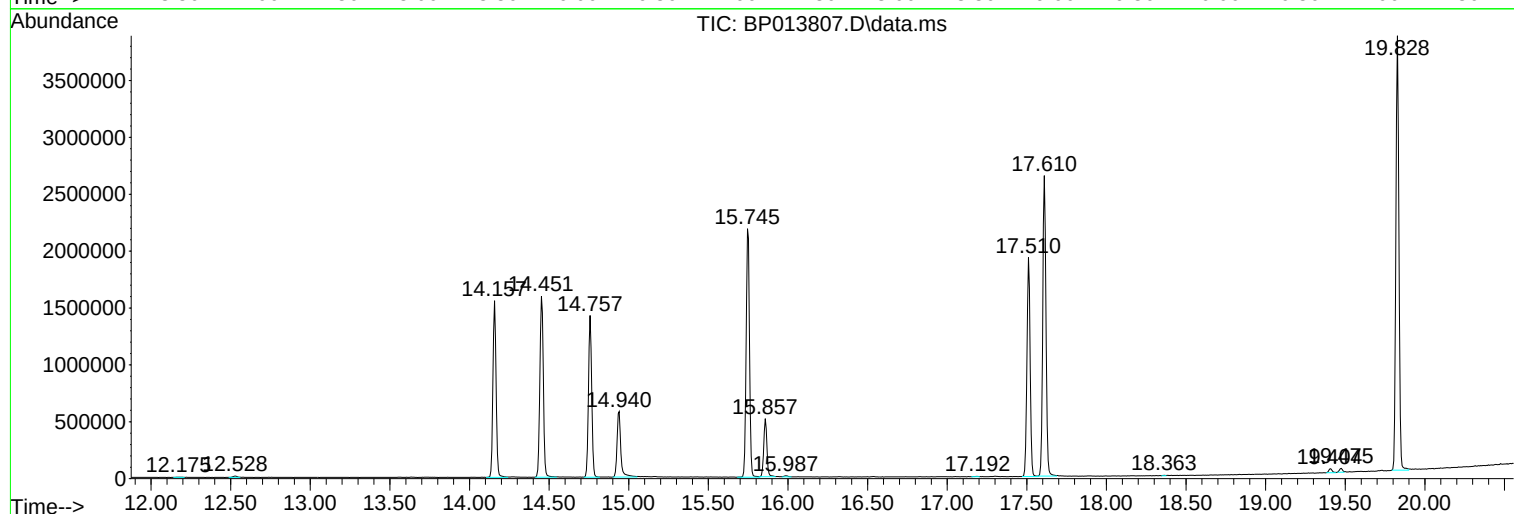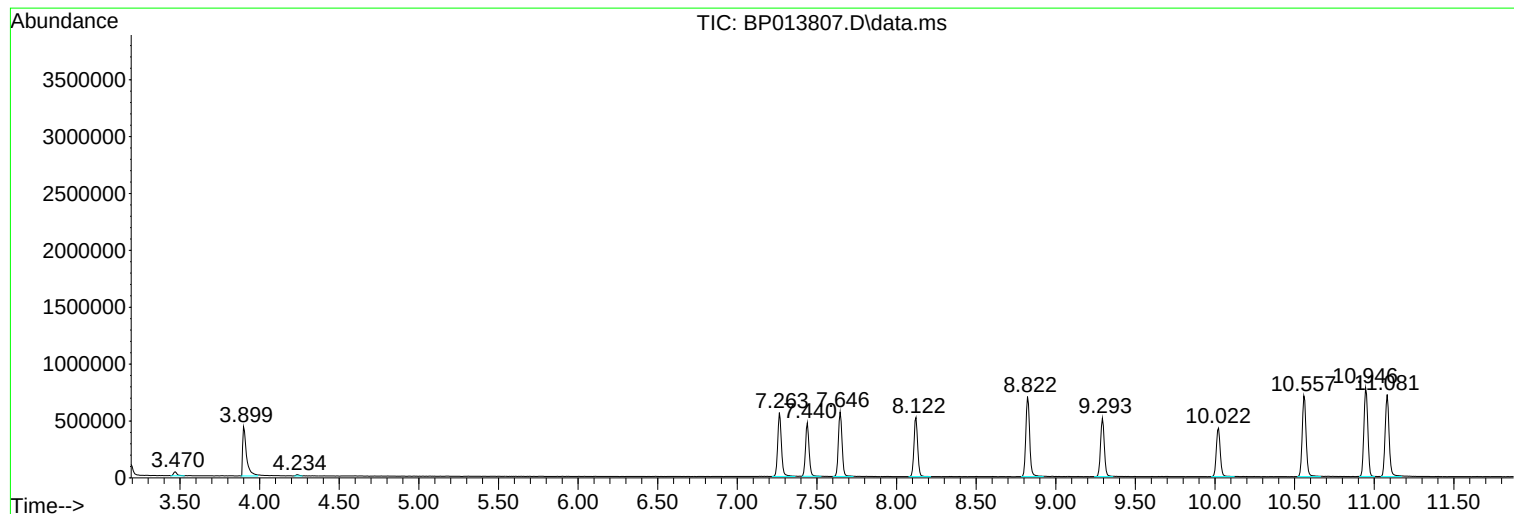

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020923\
Data File : BP013807.D
Acq On : 09 Feb 2023 09:51
Operator : CG/JU
Sample : PB150744BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK744

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020923\
Data File : BP013807.D
Acq On : 09 Feb 2023 09:51
Operator : CG/JU
Sample : PB150744BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK744

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc