

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020923\
 Data File : BP013810.D
 Acq On : 09 Feb 2023 12:22
 Operator : CG/JU
 Sample : 01381-04RX
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44M8RX

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP013810.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.469	44	48	56	rBV	29271	41191	0.71%	0.092%
2	3.905	120	122	135	rBV	122031	198831	3.43%	0.442%
3	4.140	157	162	167	rVB2	12415	20789	0.36%	0.046%
4	4.240	175	179	184	rVB	12307	18177	0.31%	0.040%
5	5.399	369	376	381	rBV	25748	44505	0.77%	0.099%
6	5.575	402	406	416	rBV3	12093	30535	0.53%	0.068%
7	7.269	691	694	702	rVB2	8507	14925	0.26%	0.033%
8	7.440	714	723	734	rBV	418894	682994	11.77%	1.519%
9	7.646	751	758	769	rBV	87232	157279	2.71%	0.350%
10	8.122	830	839	854	rBV	686985	1144888	19.74%	2.546%
11	8.481	896	900	906	rVB2	17394	26555	0.46%	0.059%
12	8.828	954	959	969	rVB2	34461	64851	1.12%	0.144%
13	9.016	988	991	997	rBV6	6309	11959	0.21%	0.027%
14	9.293	1030	1038	1049	rBV	479857	799101	13.78%	1.777%
15	9.393	1052	1055	1063	rVB10	4943	9872	0.17%	0.022%
16	9.693	1101	1106	1111	rBV3	8792	15893	0.27%	0.035%
17	9.751	1111	1116	1124	rVB4	11864	20598	0.36%	0.046%
18	10.022	1155	1162	1173	rBV2	20188	40024	0.69%	0.089%
19	10.210	1189	1194	1201	rBV6	12324	23892	0.41%	0.053%
20	10.363	1211	1220	1226	rVB6	4793	10209	0.18%	0.023%
21	10.563	1246	1254	1263	rBV	139792	264466	4.56%	0.588%
22	10.716	1273	1280	1284	rBV7	4996	8127	0.14%	0.018%
23	10.810	1288	1296	1299	rBV10	4283	8681	0.15%	0.019%
24	10.946	1309	1319	1328	rBV	1031379	1738607	29.97%	3.867%
25	11.081	1335	1342	1360	rBV	598289	1065200	18.36%	2.369%
26	11.328	1382	1384	1393	rVB10	3459	7211	0.12%	0.016%
27	11.610	1425	1432	1437	rBV	9415	19248	0.33%	0.043%
28	12.087	1507	1513	1515	rBV6	5539	7823	0.13%	0.017%
29	12.192	1524	1531	1535	rBV2	20420	36605	0.63%	0.081%
30	12.340	1551	1556	1560	rBV7	3562	6786	0.12%	0.015%
31	12.463	1568	1577	1582	rBV5	7503	15632	0.27%	0.035%
32	12.522	1582	1587	1597	rVB	14161	24703	0.43%	0.055%
33	13.169	1690	1697	1700	rBV5	6979	14272	0.25%	0.032%
34	13.569	1759	1765	1768	rBV7	3448	6076	0.10%	0.014%
35	13.639	1773	1777	1784	rVB3	12594	20150	0.35%	0.045%
36	14.063	1844	1849	1853	rBV8	8535	14237	0.25%	0.032%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020923\
 Data File : BP013810.D
 Acq On : 09 Feb 2023 12:22
 Operator : CG/JU
 Sample : 01381-04RX
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 A44M8RX

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
 Title : SVOA CALIBRATION

37	14.157	1857	1865	1879	rBV	1247542	1758237	30.31%	3.911%
38	14.275	1881	1885	1890	rVB8	5147	9876	0.17%	0.022%
39	14.451	1908	1915	1929	rBV	1820121	2646630	45.62%	5.887%
40	14.757	1959	1967	1975	rBV	1835346	2687329	46.33%	5.977%
41	15.004	2004	2009	2017	rBV4	11032	22803	0.39%	0.051%
42	15.163	2033	2036	2041	rVB7	5073	6717	0.12%	0.015%
43	15.745	2125	2135	2152	rBV	2500537	3747691	64.60%	8.336%
44	15.986	2171	2176	2182	rVB3	13143	20311	0.35%	0.045%
45	16.110	2193	2197	2201	rBV	12790	17417	0.30%	0.039%
46	16.963	2338	2342	2345	rBV6	6136	9629	0.17%	0.021%
47	17.251	2387	2391	2394	rBV6	6323	8503	0.15%	0.019%
48	17.298	2394	2399	2403	rBV5	9743	19452	0.34%	0.043%
49	17.510	2428	2435	2445	rBV	2599359	3756024	64.75%	8.354%
50	17.610	2445	2452	2462	rVV	3265846	4536306	78.20%	10.090%
51	18.363	2577	2580	2585	rBV7	11505	16878	0.29%	0.038%
52	19.404	2754	2757	2762	rVB2	49046	63686	1.10%	0.142%
53	19.469	2765	2768	2772	rBV	42021	57473	0.99%	0.128%
54	19.827	2823	2829	2840	rBV	4271620	5801014	100.00%	12.903%
55	21.257	3069	3072	3079	rBV5	86847	144846	2.50%	0.322%
56	21.586	3123	3128	3138	rVB	3155955	4182951	72.11%	9.304%
57	23.980	3528	3535	3551	rVB2	2393782	5098338	87.89%	11.340%
58	24.151	3557	3564	3574	rVB2	1725514	3712418	64.00%	8.257%




Sum of corrected areas: 44959421

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020923\
Data File : BP013810.D
Acq On : 09 Feb 2023 12:22
Operator : CG/JU
Sample : 01381-04RX
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44M8RX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

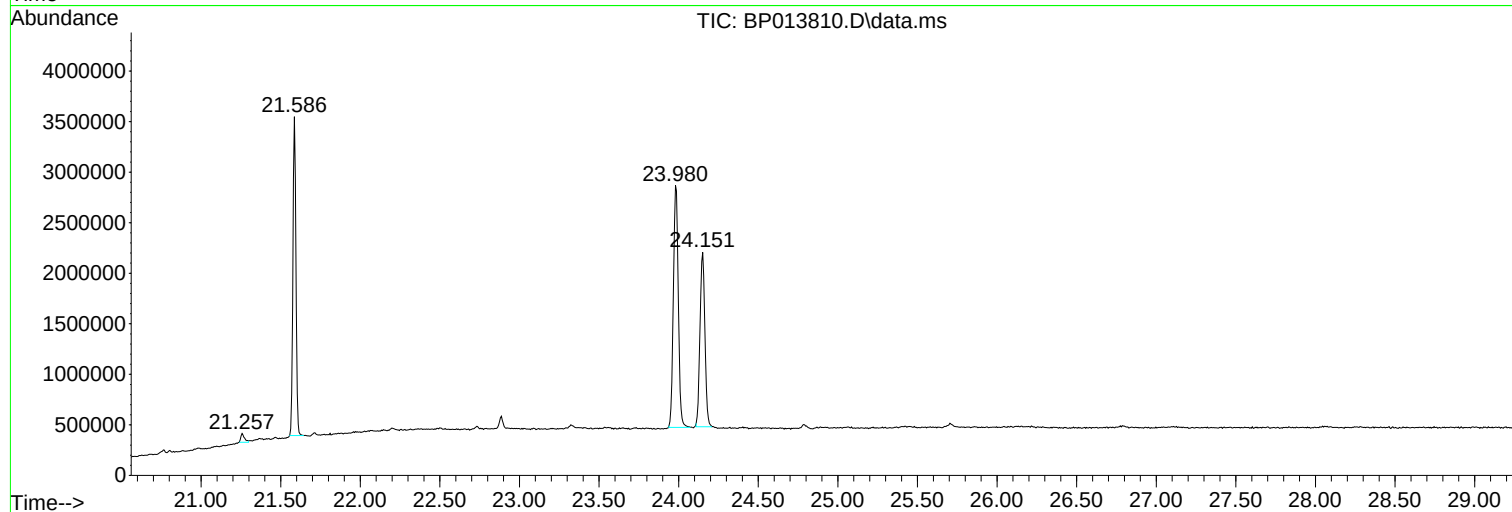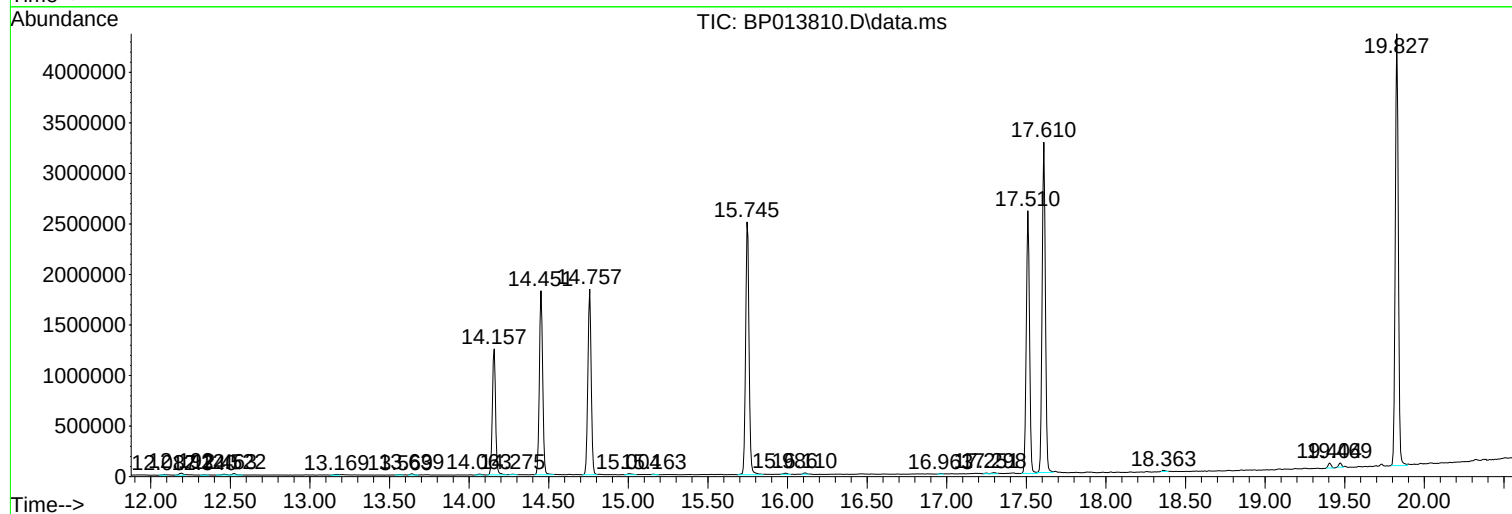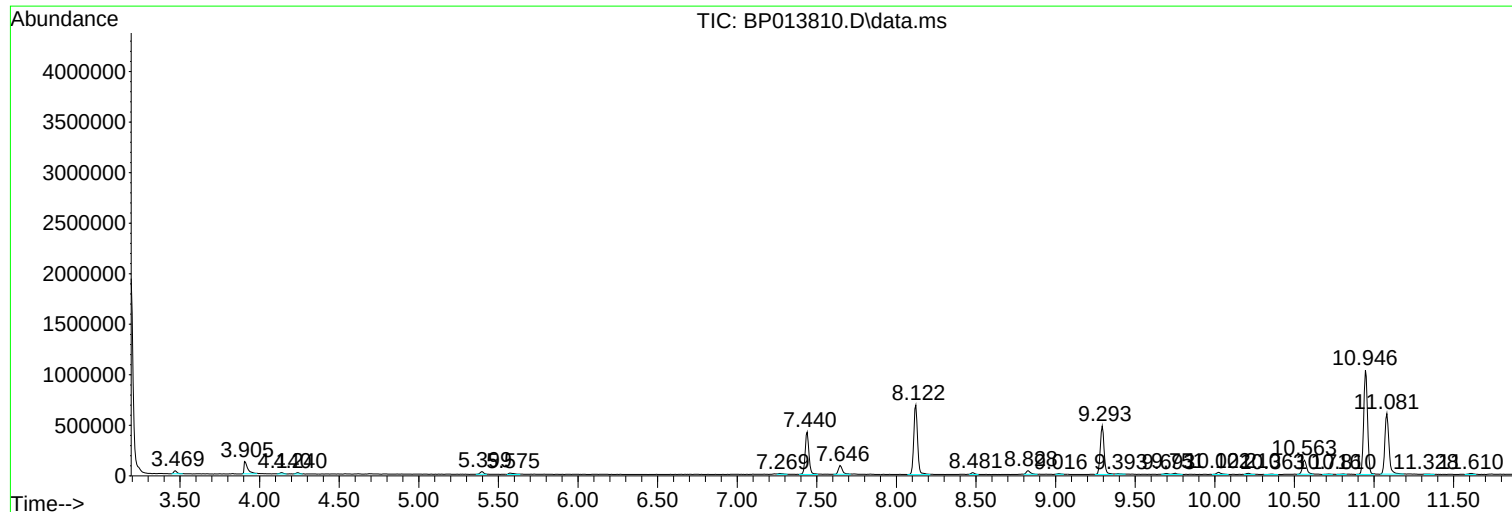

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020923\
Data File : BP013810.D
Acq On : 09 Feb 2023 12:22
Operator : CG/JU
Sample : 01381-04RX
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44M8RX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP020923\
Data File : BP013810.D
Acq On : 09 Feb 2023 12:22
Operator : CG/JU
Sample : 01381-04RX
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
A44M8RX

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP020723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc