
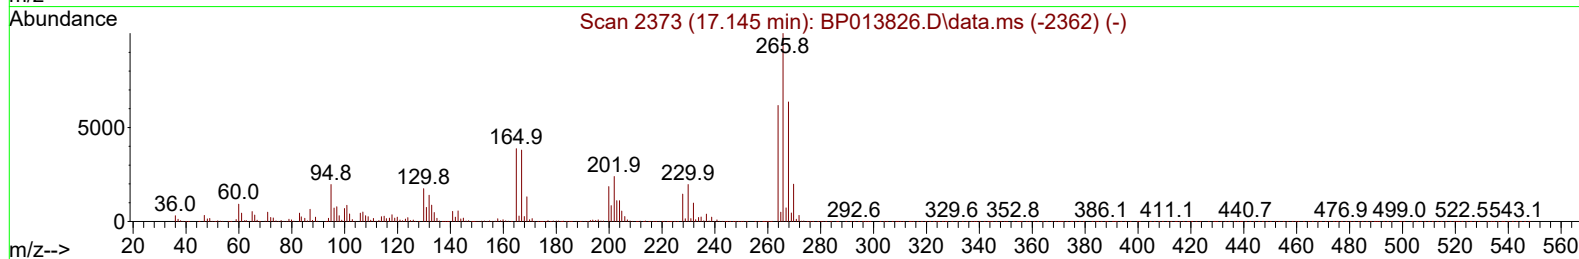
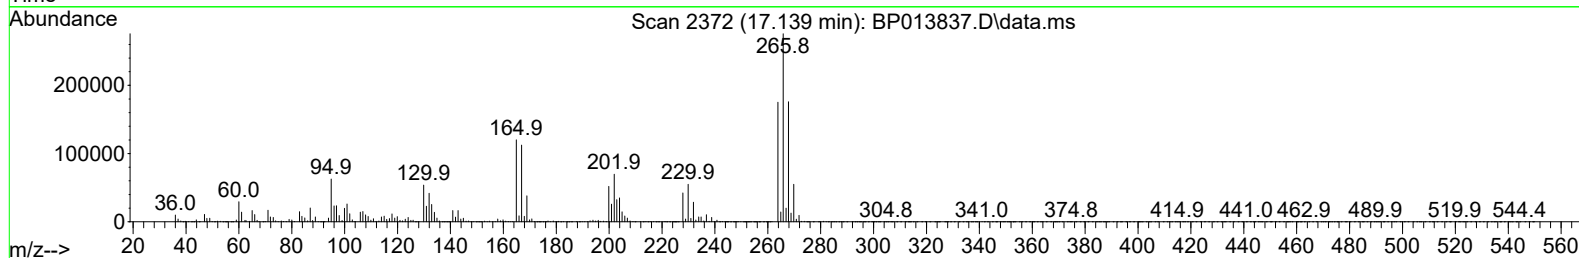


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021723\
Data File : BP013837.D
Acq On : 17 Feb 2023 09:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 04:40:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 18:05:40 2023
Response via : Initial Calibration

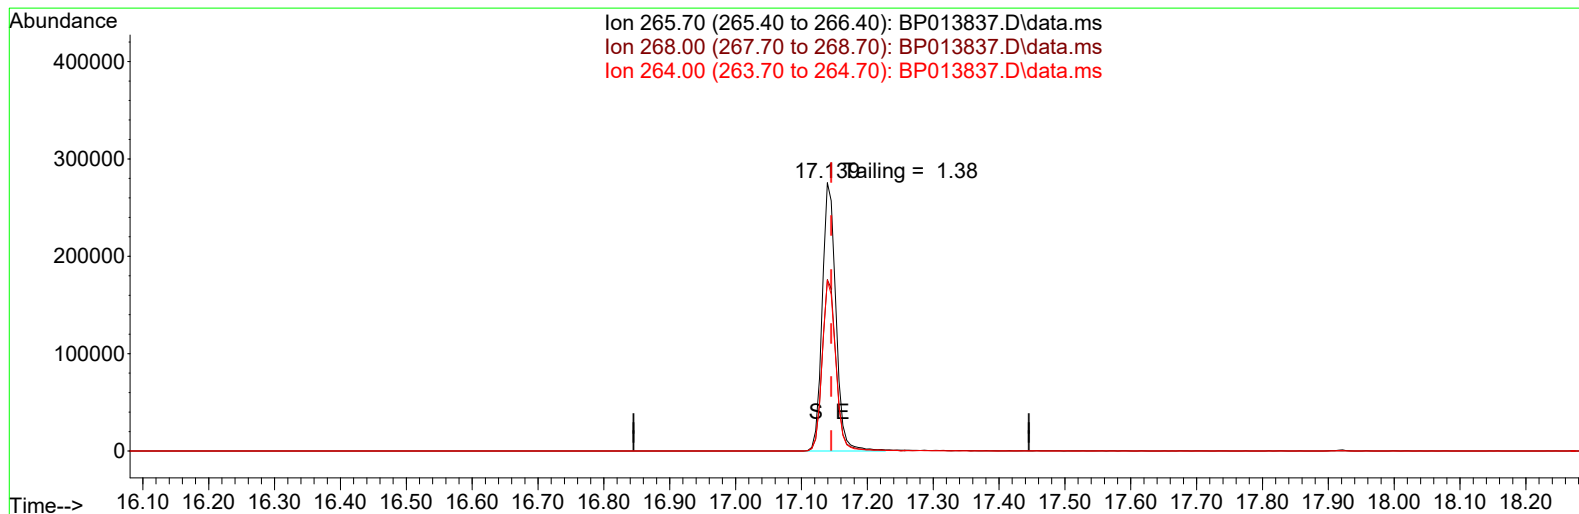

TIC: BP013837.D\data.ms

(70) Pentachlorophenol (C)




17.139min (-0.006) 656184.68 ng

response 398924

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.85
264.00	61.70	63.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021723\
Data File : BP013837.D
Acq On : 17 Feb 2023 09:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Feb 18 04:40:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 18:05:40 2023
Response via : Initial Calibration

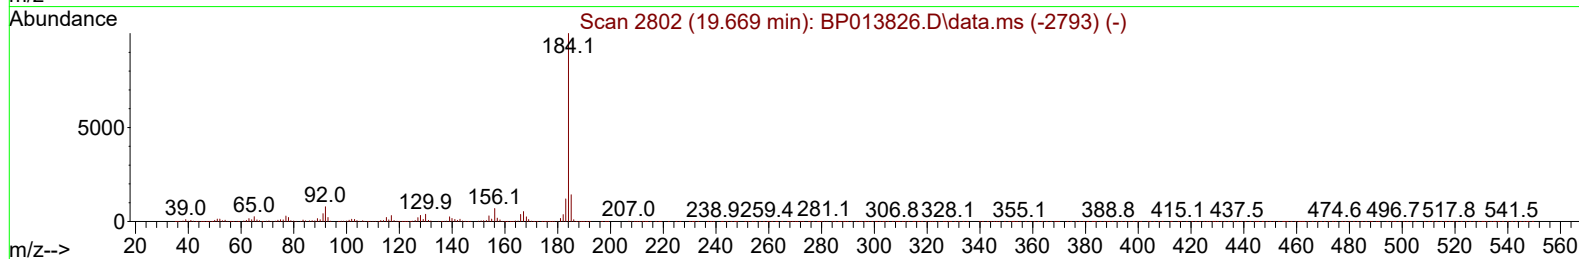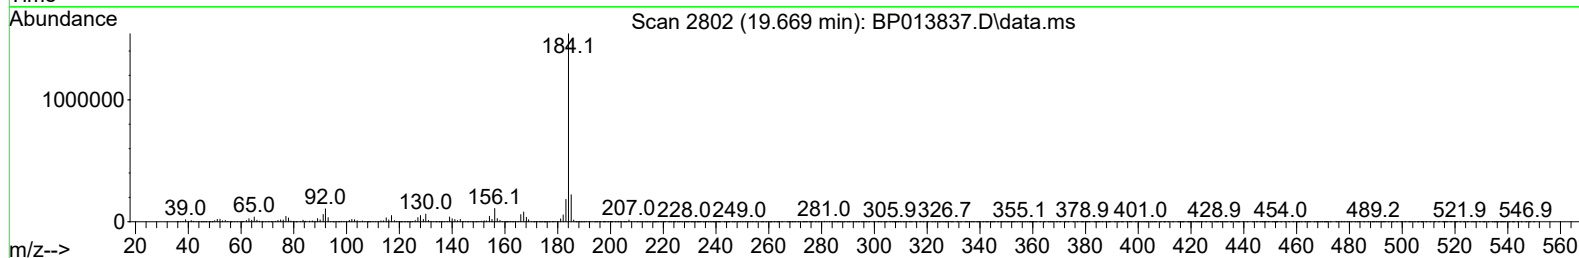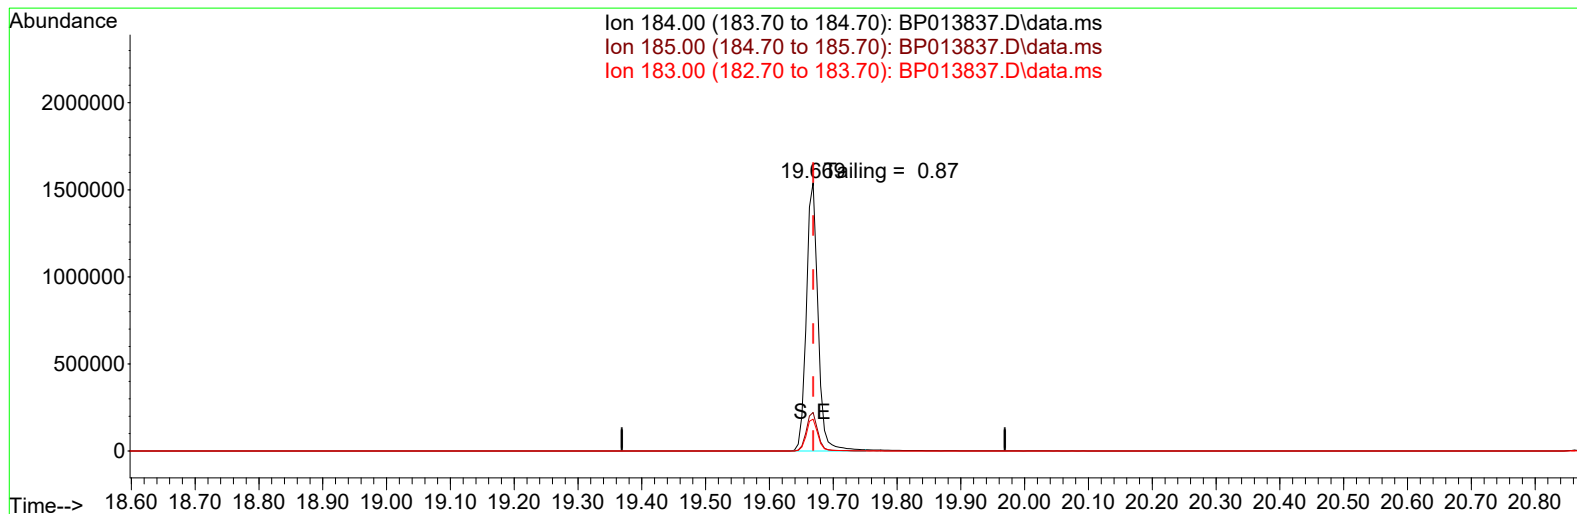

TIC: BP013837.D\data.ms

(77) Benzidine**19.669min (-0.000) 4884763.15 ng****response 1991397**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.37
183.00	12.00	11.89
0.00	0.00	0.00