
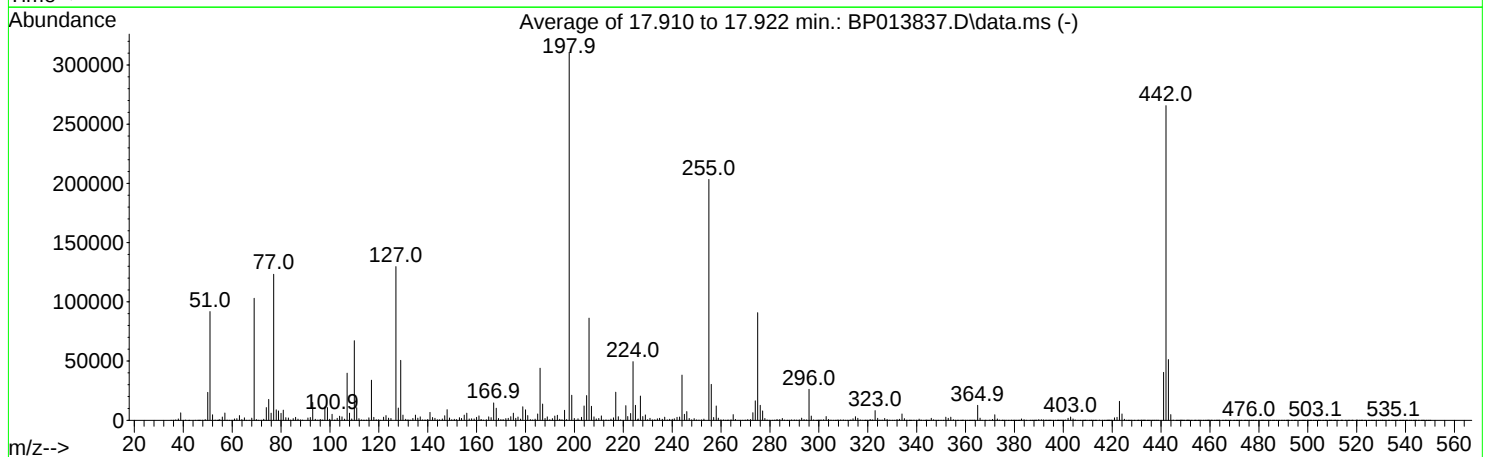


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021723\
Data File : BP013837.D
Acq On : 17 Feb 2023 09:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Feb 17 18:05:40 2023

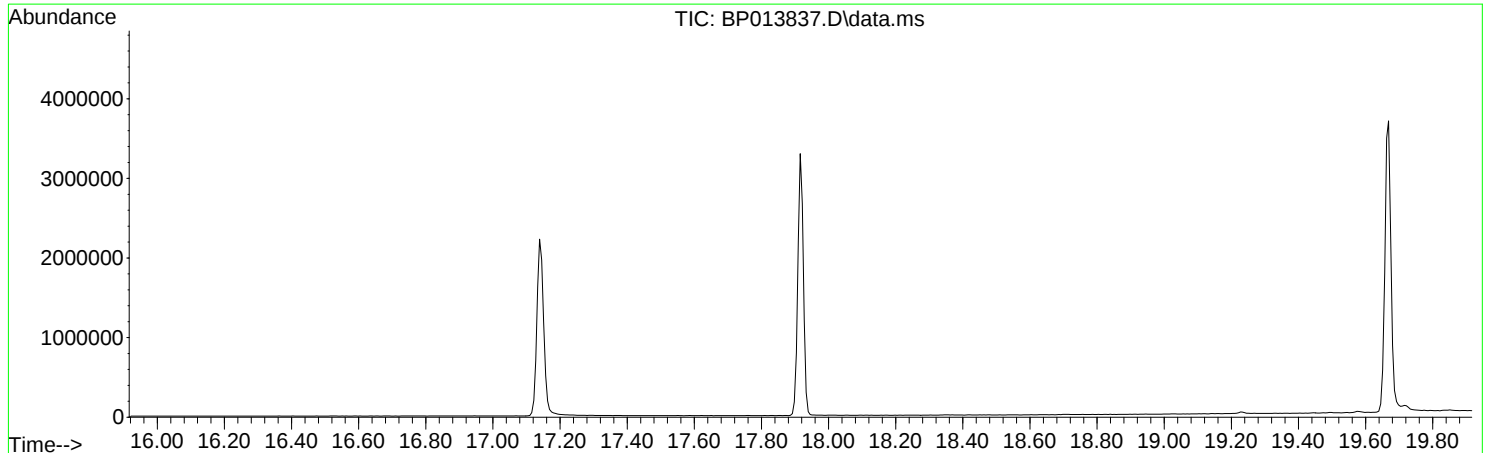




AutoFind: Scans 2503, 2504, 2505; Background Corrected with Scan 2495

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.5	91739	PASS
68	69	0.00	2	1.8	1822	PASS
69	198	0.00	100	33.2	103067	PASS
70	69	0.00	2	0.6	641	PASS
127	198	10	80	41.8	129795	PASS
197	198	0.00	2	0.2	606	PASS
198	198	100	100	100.0	310566	PASS
199	198	5	9	6.8	21154	PASS
275	198	10	60	29.3	90904	PASS
365	198	1	100	4.1	12673	PASS
441	198	0.01	100	13.0	40483	PASS
442	442	100	100	100.0	265657	PASS
443	442	15	24	19.3	51277	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021723\
Data File : BP013837.D
Acq On : 17 Feb 2023 09:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Feb 18 04:40:04 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 17 18:05:40 2023
Response via : Initial Calibration

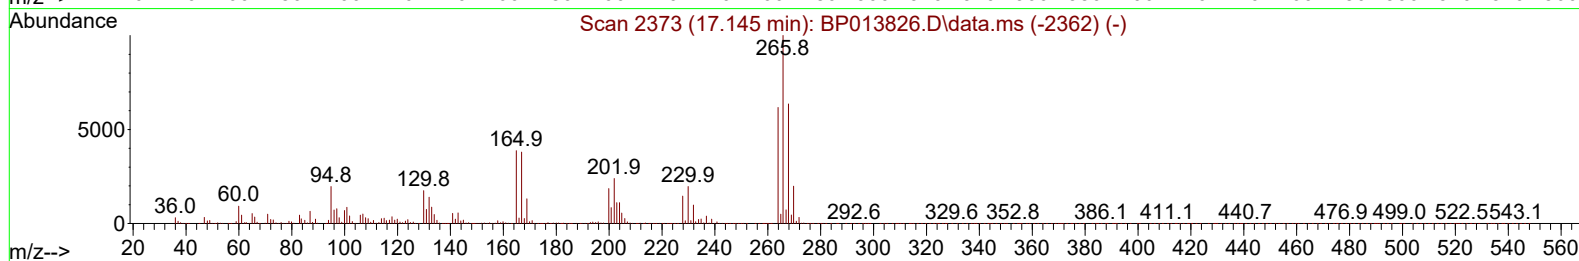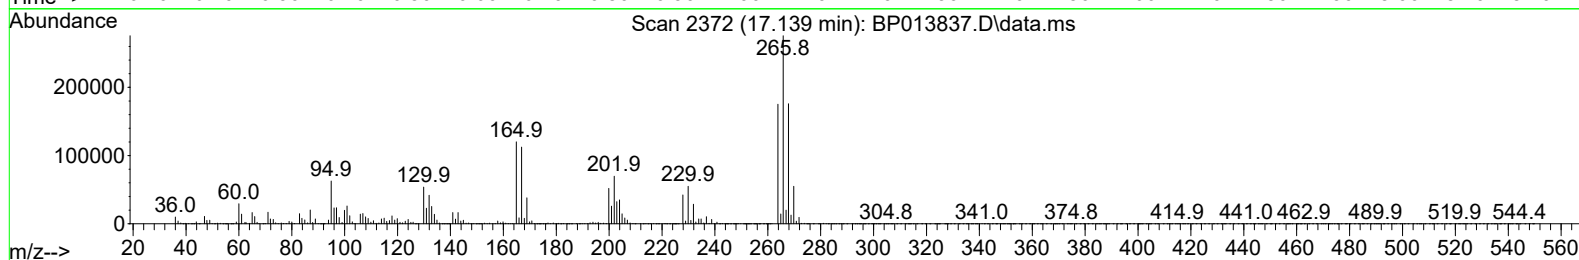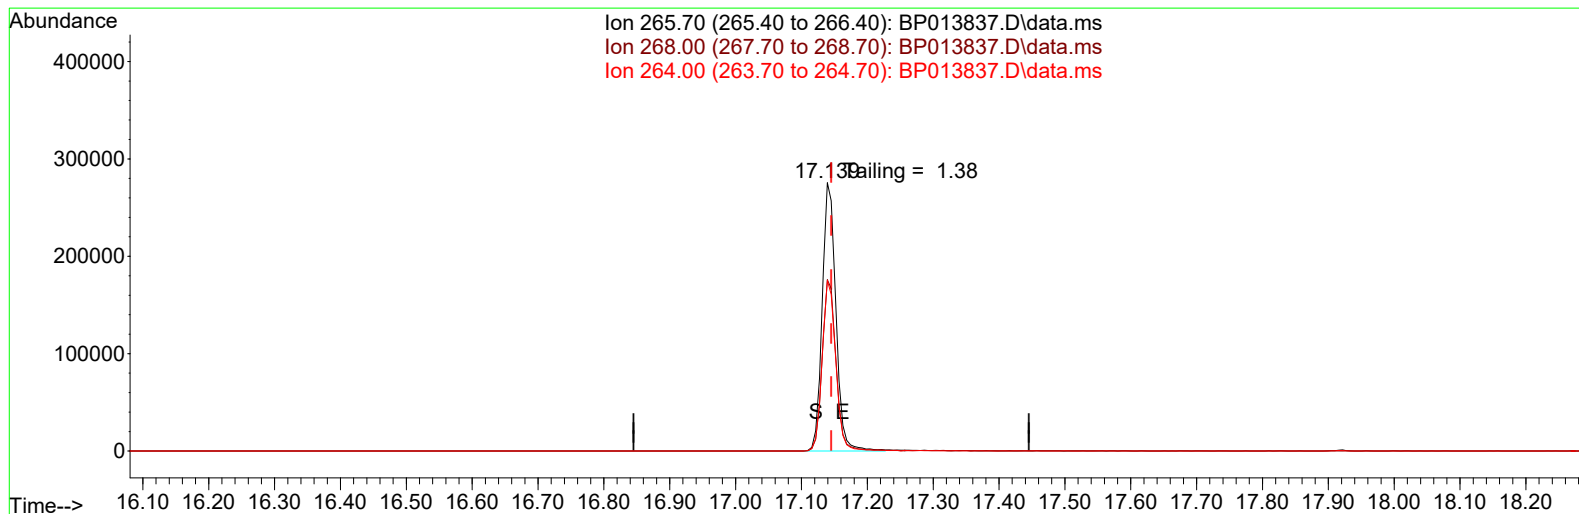

TIC: BP013837.D\data.ms

(70) Pentachlorophenol (C)

17.139min (-0.006) 656184.68 ng




response 398924

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.85
264.00	61.70	63.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP021723\
 Data File : BP013837.D
 Acq On : 17 Feb 2023 09:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Feb 18 04:40:04 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 17 18:05:40 2023
 Response via : Initial Calibration

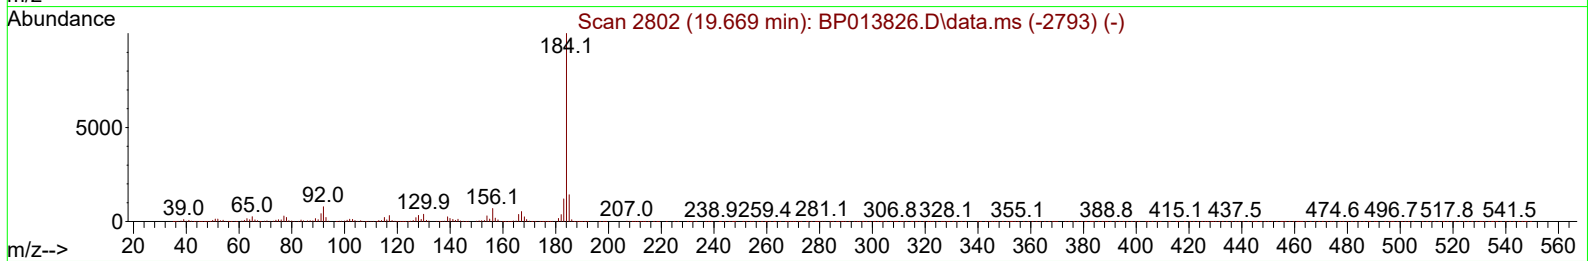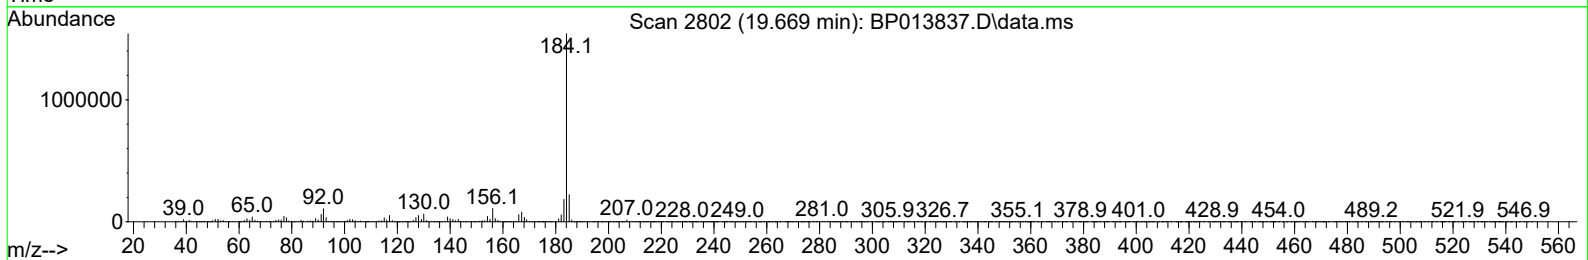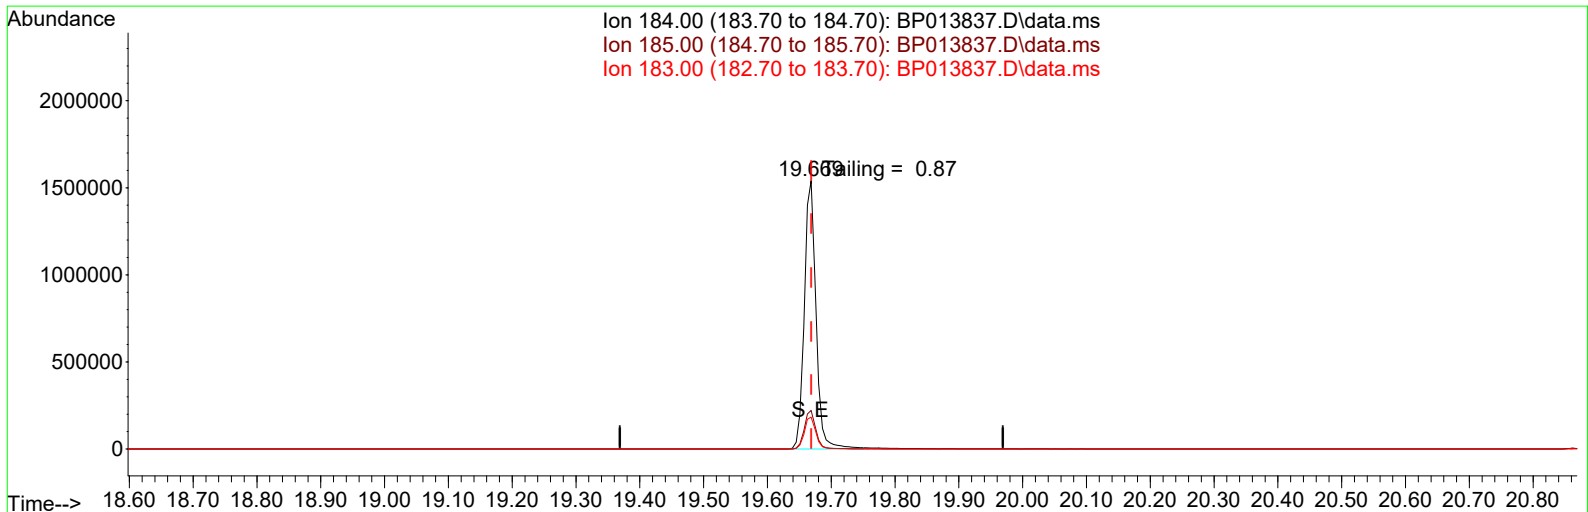

TIC: BP013837.D\data.ms

(77) Benzidine

19.669min (-0.000) 4884763.15 ng

response 1991397

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.37
183.00	12.00	11.89
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/17/2023	BNA_P	<u>BP013837.D</u>
Compound Name	Response	Retention Time
DDT	1028491	20.863
DDD	12116	20.486
DDE	834	19.939
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12950	1041441	1.24

Instrument :
BNA_P
ClientSampleId :
DFTPP