
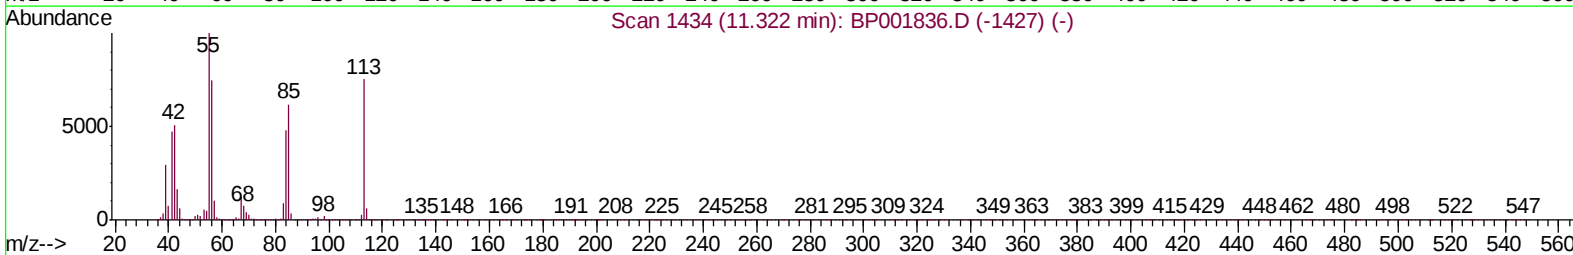
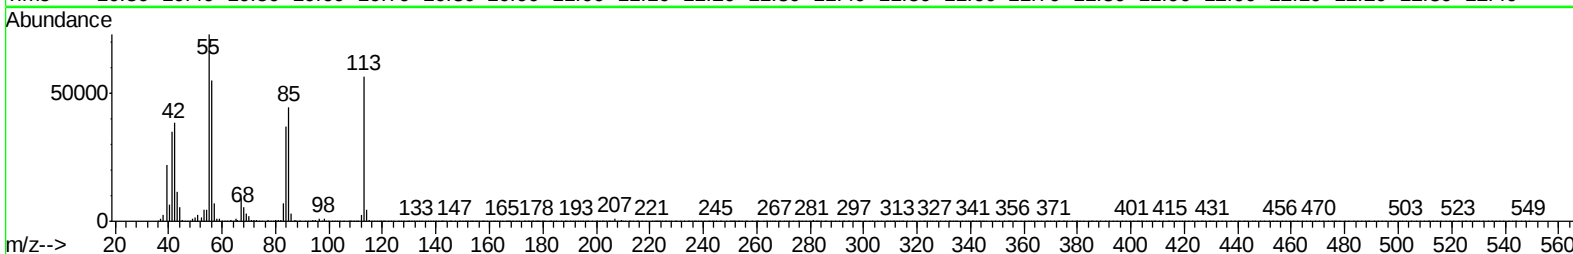


Data File : BP001851.D
Acq On : 22 Feb 2020 07:25
Operator : CG/JU
Sample : SSTDCCC020EC
Misc :
ALS Vial : 31 Sample Multiplier: 1

Quant Time: Feb 24 01:14:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 01:10:13 2020
Response via : Initial Calibration

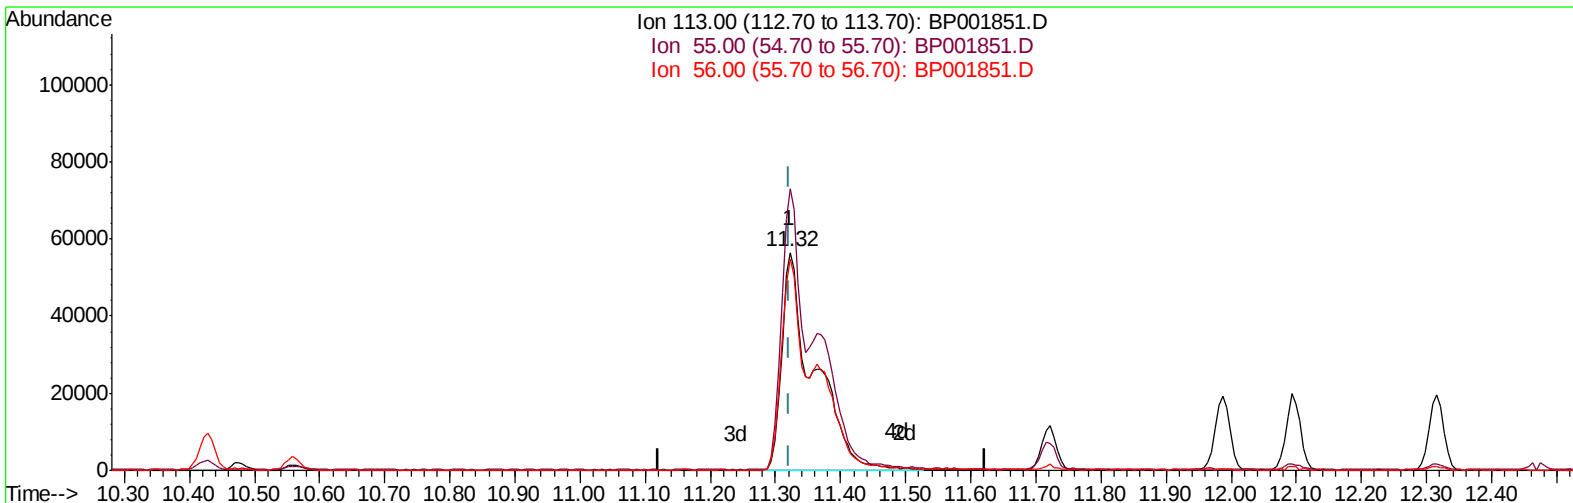

TIC: BP001851.D

(32) Caprolactam

11.322min (-0.000) 24.11ng/ul m

response 194775

Ion	Exp%	Act%
113.00	100	100
55.00	138.80	129.11
56.00	107.70	97.06
0.00	0.00	0.00