

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022120\
 Data File : BP001822.D
 Acq On : 21 Feb 2020 14:33
 Operator : CG/JU
 Sample : L1555-04
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBD83

Quant Time: Feb 21 15:13:35 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 21 07:12:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.66	152	449010	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1881734	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1232790	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2759819	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2763926	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	3089743	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.18	96	54261	5.02	ng/uL	0.00
5) Phenol-d5	6.83	99	211553	6.24	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	553881	28.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	685809	25.01	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	414588	15.41	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	421080	33.06	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	476009	41.32	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	810275	29.58	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	49192	1.52	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	3022038	34.93	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	3459449	32.47	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	105528	7.01	ng/ul	0.00
58) Fluorene-d10	15.29	176	2637787	33.90	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	457524	42.05	ng/ul	0.00
71) Anthracene-d10	17.14	188	4345531	35.74	ng/ul	0.00
79) Pyrene-d10	19.39	212	5044174	35.56	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	5625033	37.70	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.75	163	178086	1.956	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022120\
Data File : BP001822.D
Acq On : 21 Feb 2020 14:33
Operator : CG/JU
Sample : L1555-04
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBD83

Quant Time: Feb 21 15:13:35 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 21 07:12:24 2020
Response via : Initial Calibration

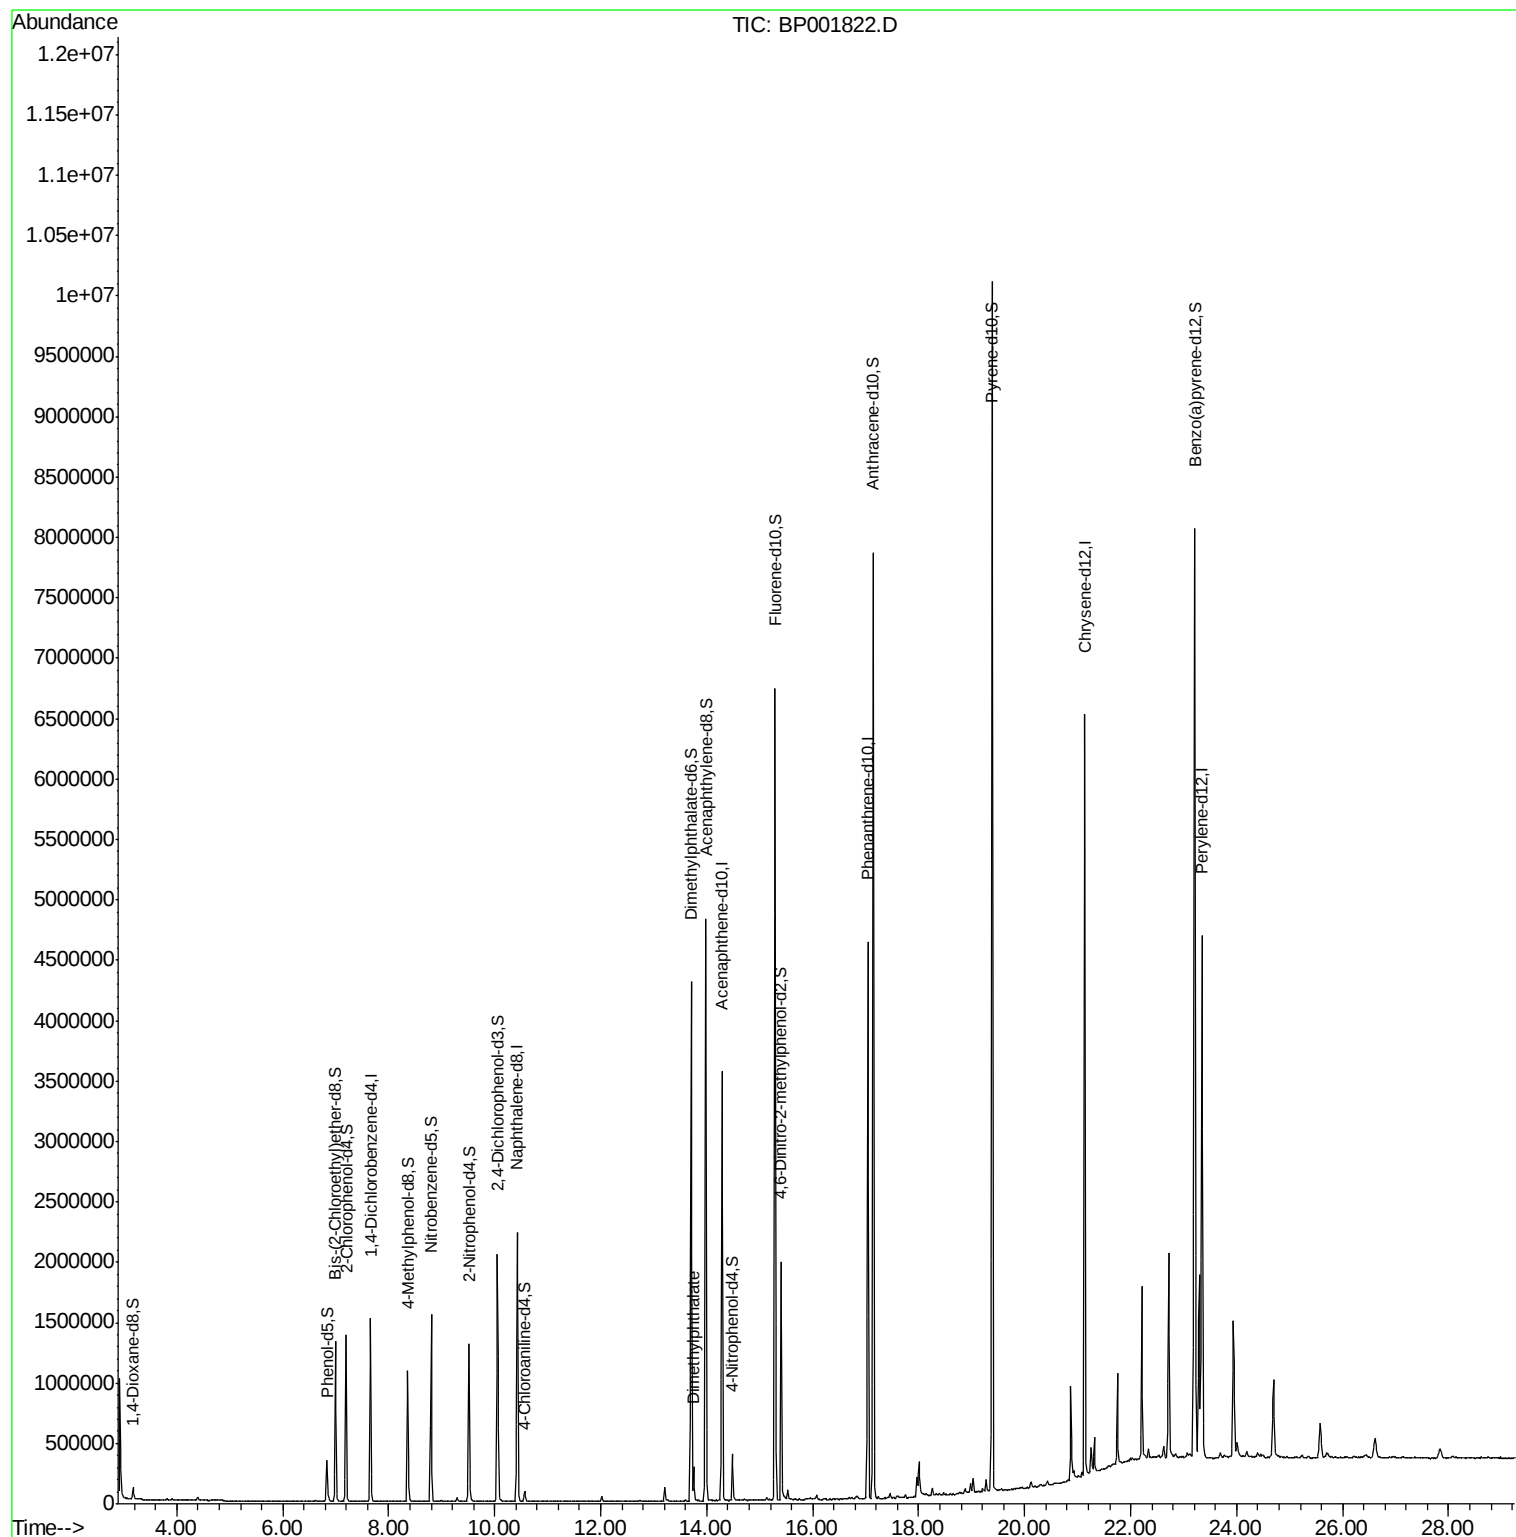

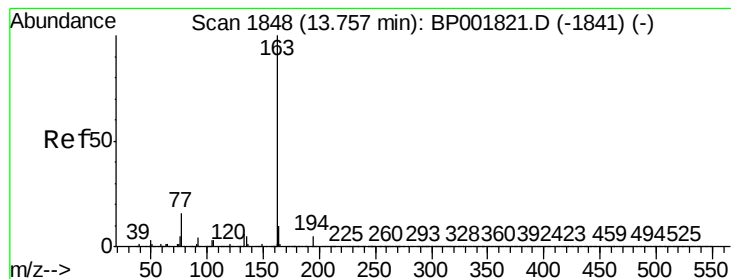

#45

Dimethylphthalate

Concen: 1.956 ng/ul

RT: 13.75 min Scan# 1847

Delta R.T. -0.01 min

Lab File: BP001822.D

Acq: 21 Feb 2020 14:33

Instrument :

BNA_P

ClientSampleId :

DBD83

Tot Ion:163 Resp: 178086

Ion Ratio Lower Upper

163 100

194 4.0 3.5 5.3

164 9.7 8.0 12.0

