

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022120\
 Data File : BP001823.D
 Acq On : 21 Feb 2020 15:07
 Operator : CG/JU
 Sample : L1555-05
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBD87

Quant Time: Feb 21 15:38:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 21 07:12:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	486156	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	2000804	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1301452	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2921491	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2864960	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	3196214	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.18	96	77409	6.61	ng/uL	0.00
5) Phenol-d5	6.83	99	292830	7.97	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	641311	30.05	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	833000	28.06	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	544024	18.67	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	491590	36.29	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	553943	45.22	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	969801	33.30	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	57463	1.67	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	3470950	38.00	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	3957274	35.19	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	138554	8.71	ng/ul	0.00
58) Fluorene-d10	15.29	176	3016121	36.72	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	519882	45.14	ng/ul	0.00
71) Anthracene-d10	17.14	188	4782809	37.16	ng/ul	0.00
79) Pyrene-d10	19.39	212	5458823	37.13	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	6061900	39.27	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.75	163	162323	1.689	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022120\
Data File : BP001823.D
Acq On : 21 Feb 2020 15:07
Operator : CG/JU
Sample : L1555-05
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBD87

Quant Time: Feb 21 15:38:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 21 07:12:24 2020
Response via : Initial Calibration

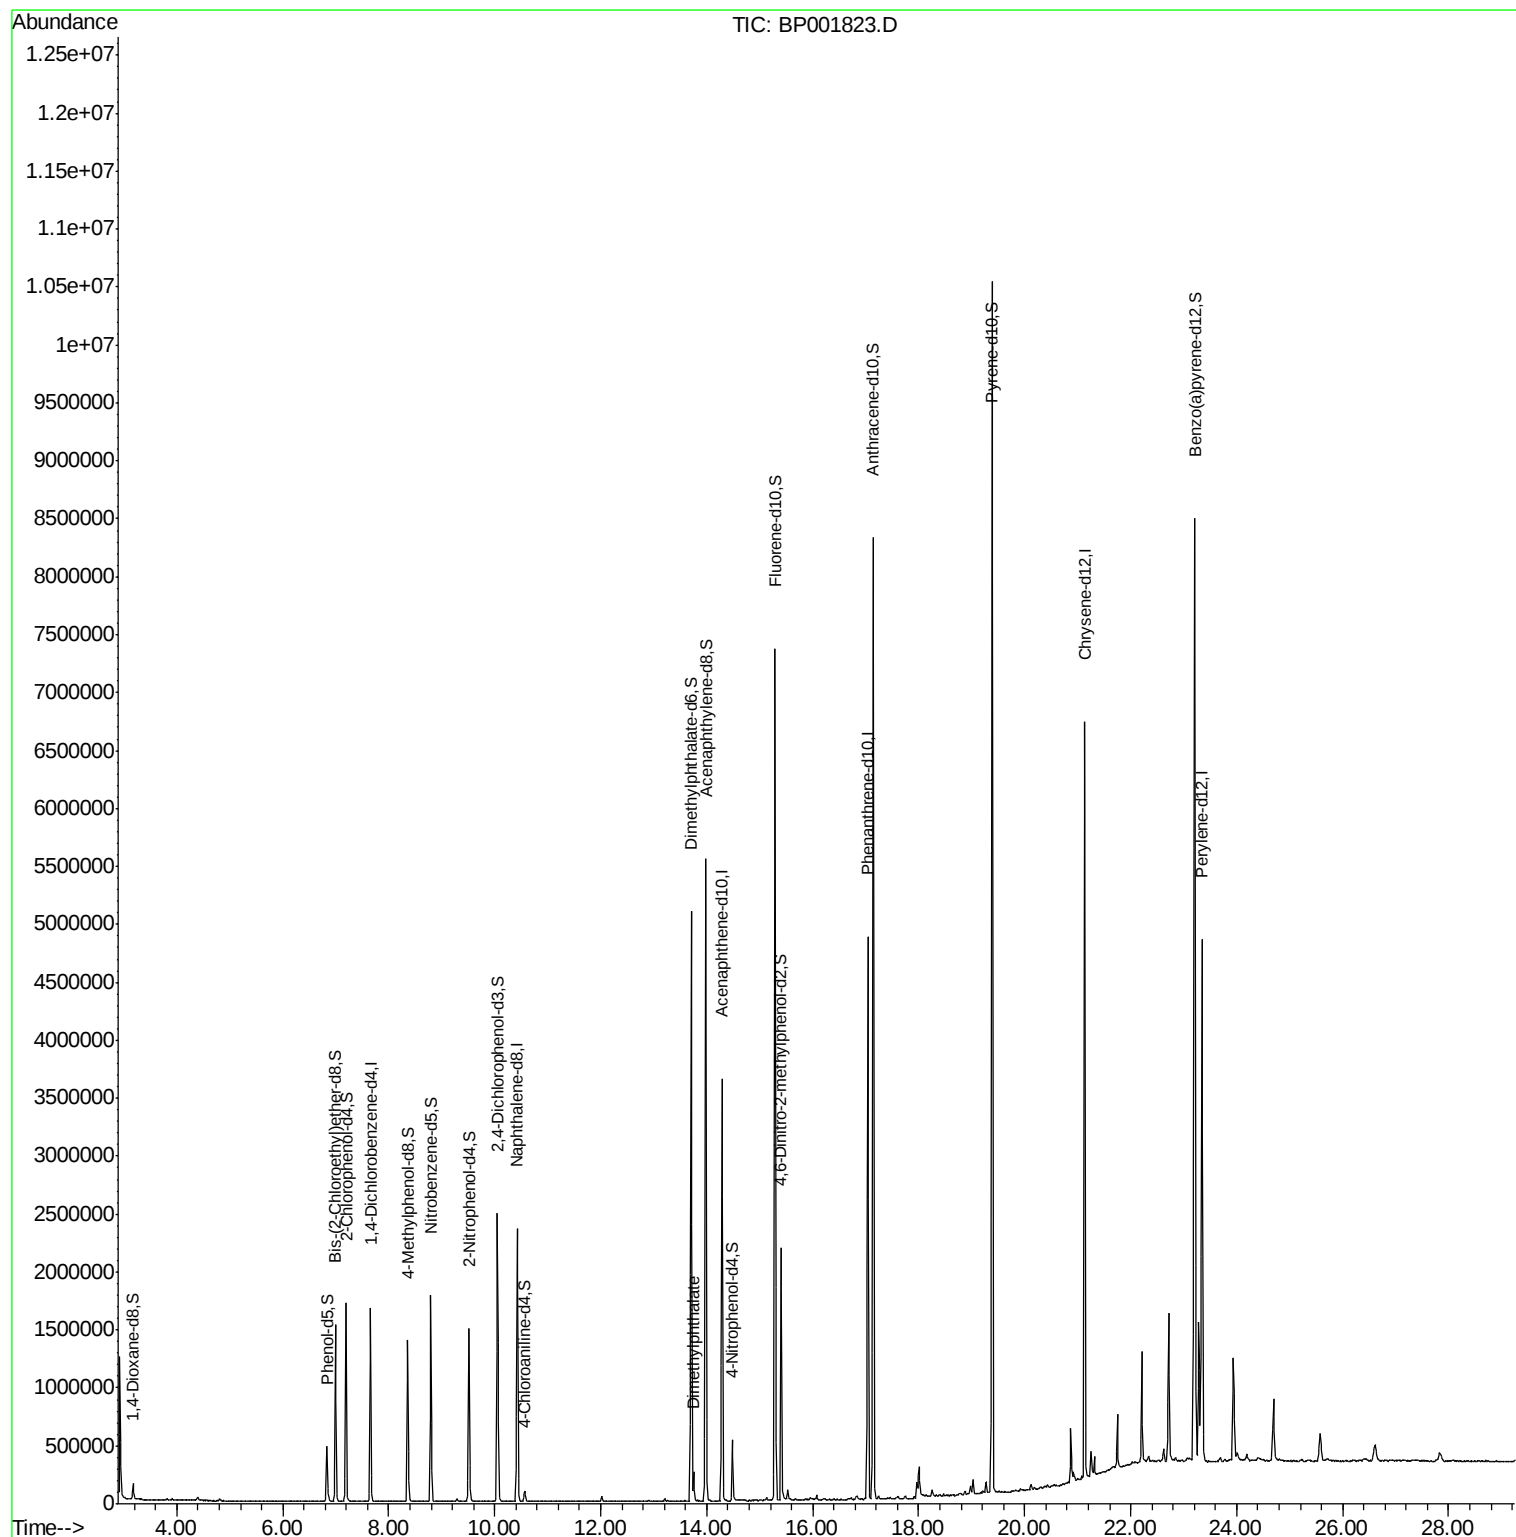

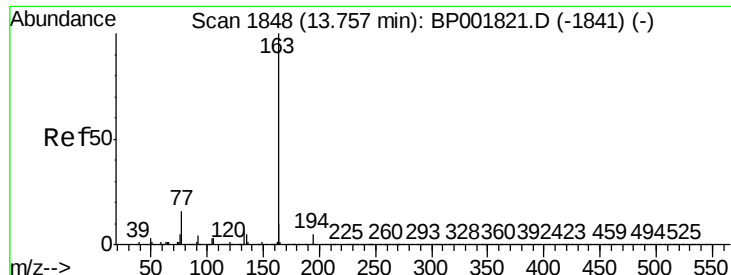

#45

Dimethylphthalate

Concen: 1.689 ng/ul

RT: 13.75 min Scan# 1847

Delta R.T. -0.01 min

Lab File: BP001823.D

Acq: 21 Feb 2020 15:07

Instrument :

BNA_P

ClientSampleId :

DBD87


Tot Ion:163 Resp: 162323

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 10.1 8.0 12.0

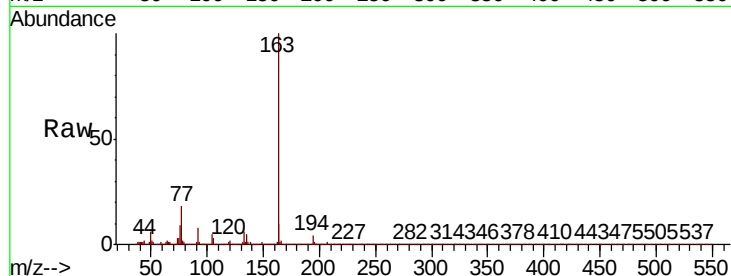

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

