

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022120\
 Data File : BP001824.D
 Acq On : 21 Feb 2020 15:41
 Operator : CG/JU
 Sample : L1555-06
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBD88

Quant Time: Feb 21 16:10:29 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Feb 21 07:12:24 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	463327	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1936520	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1254572	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2845226	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2885070	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	3250024	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.18	96	79431	7.12	ng/uL	0.00
5) Phenol-d5	6.83	99	236582	6.76	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	583506	28.69	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	740059	26.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	448985	16.17	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	450895	34.39	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	502197	42.36	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	858616	30.46	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	53712	1.61	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	3125197	35.50	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	3623406	33.42	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	105523	6.88	ng/ul	0.00
58) Fluorene-d10	15.29	176	2749034	34.72	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	456006	40.65	ng/ul	0.00
71) Anthracene-d10	17.14	188	4348056	34.69	ng/ul	0.00
79) Pyrene-d10	19.39	212	4966976	33.55	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	5672713	36.14	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.75	163	208348	2.248	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022120\
Data File : BP001824.D
Acq On : 21 Feb 2020 15:41
Operator : CG/JU
Sample : L1555-06
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBD88

Quant Time: Feb 21 16:10:29 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Feb 21 07:12:24 2020
Response via : Initial Calibration

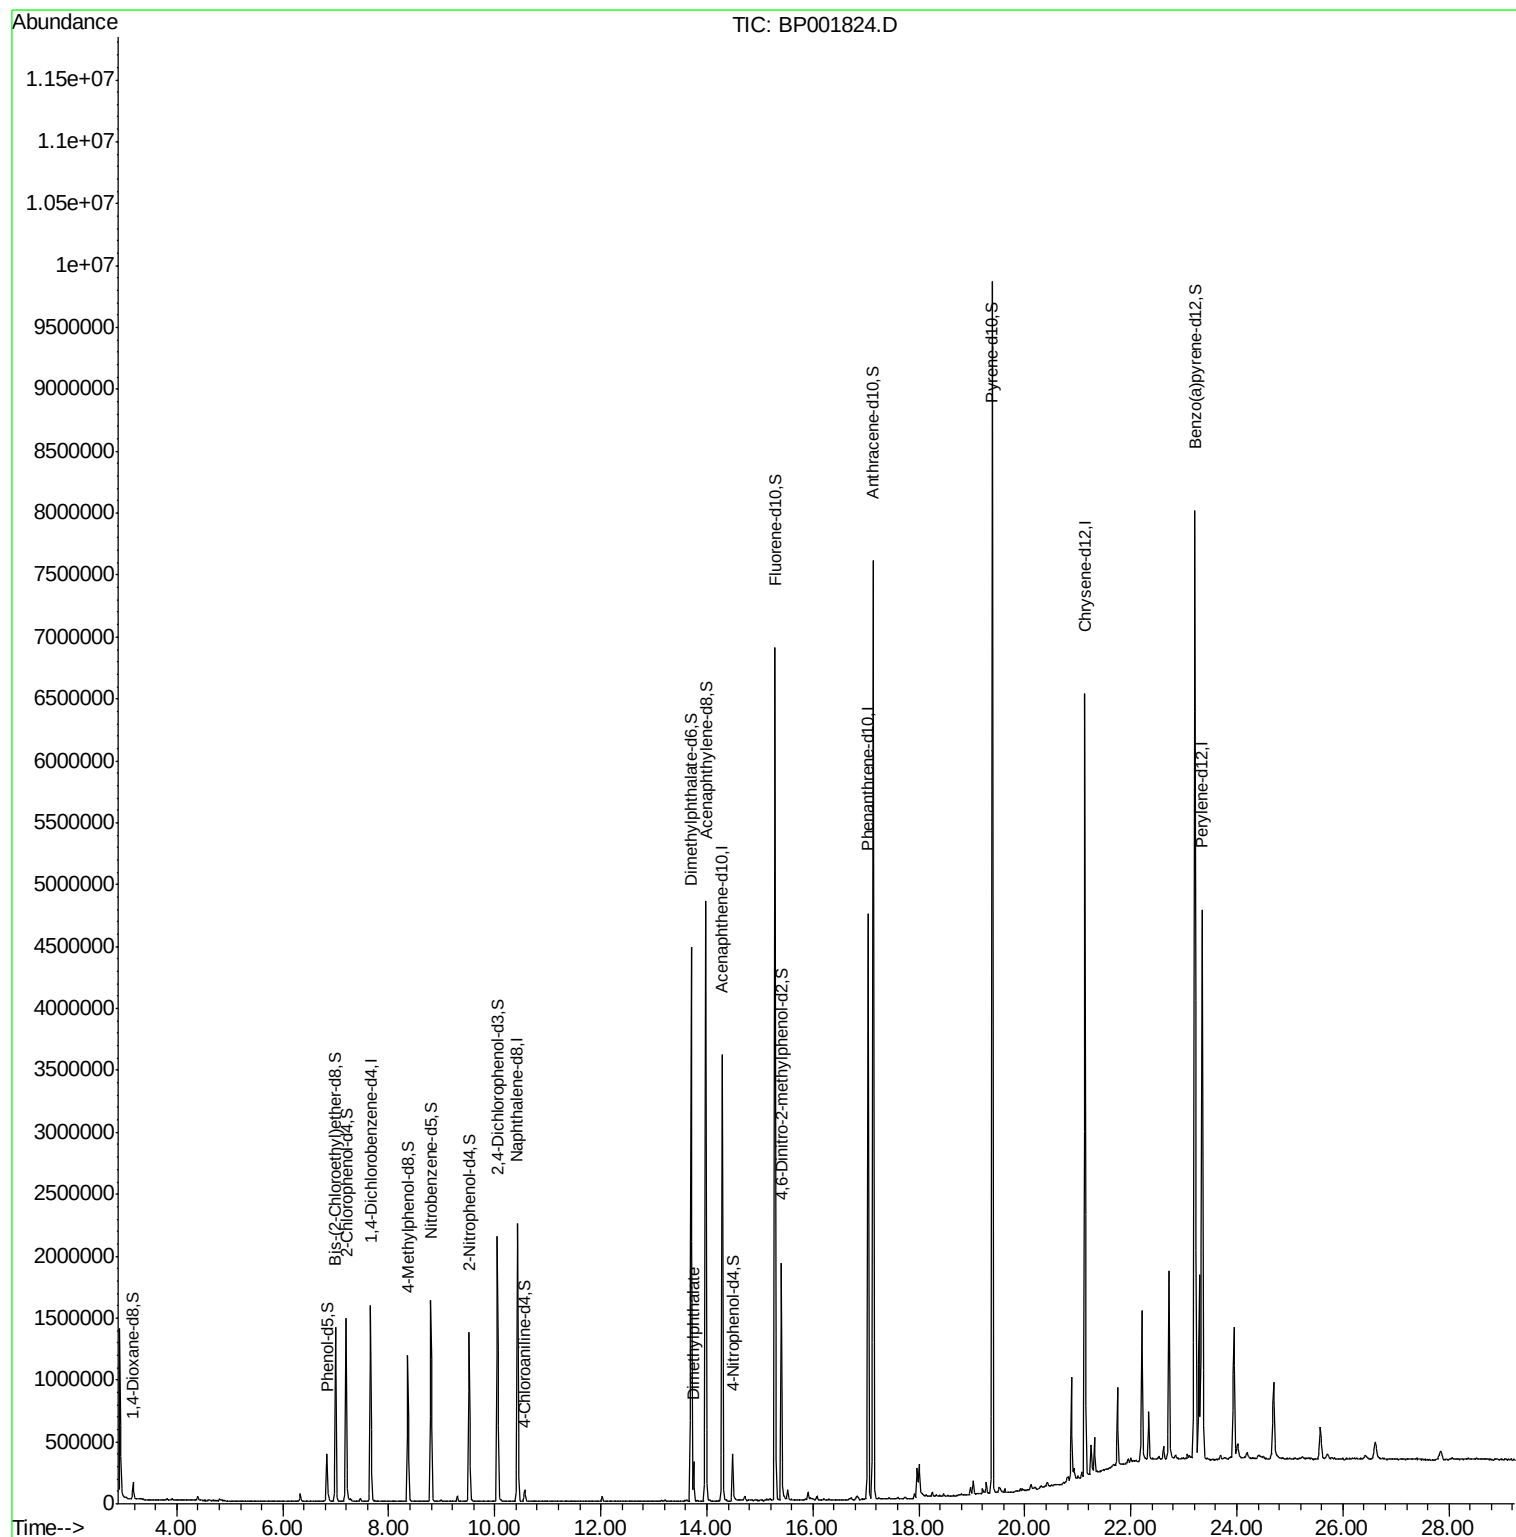

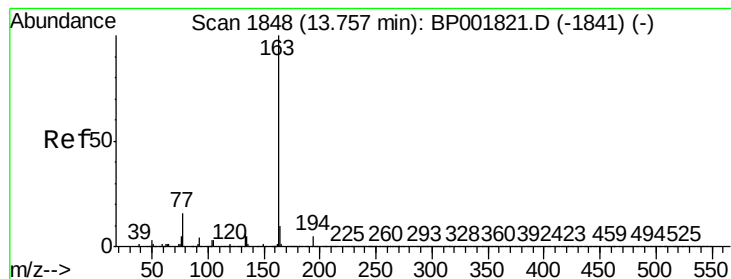

#45

Dimethylphthalate

Concen: 2.248 ng/ul

RT: 13.75 min Scan# 1847

Delta R.T. -0.01 min

Lab File: BP001824.D

Acq: 21 Feb 2020 15:41

Instrument :

BNA_P

ClientSampleId :

DBD88

Tot Ion:163 Resp: 208348

Ion Ratio Lower Upper

163 100

194 4.0 3.5 5.3

164 9.7 8.0 12.0

