

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022120\
 Data File : BP001830.D
 Acq On : 21 Feb 2020 19:03
 Operator : CG/JU
 Sample : L1506-04
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBCY2

Quant Time: Feb 22 03:46:23 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 22 03:43:48 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	322853	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1399268	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	922700	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2157398	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2227837	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	2590905	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.17	96	45142	5.81	ng/uL	0.00
5) Phenol-d5	6.83	99	864751	35.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	516110	36.42	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	777828	39.45	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	694693	35.90	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	403227	42.57	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	449535	52.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	821587	40.33	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	1134887	47.10	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	2740491	42.32	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	3248071	40.74	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	476814	42.29	ng/ul	0.00
58) Fluorene-d10	15.29	176	2423480	41.62	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	380319	44.71	ng/ul	0.00
71) Anthracene-d10	17.14	188	3730701	39.25	ng/ul	0.00
79) Pyrene-d10	19.39	212	4458010	38.99	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	5225694	41.76	ng/ul	0.00


Target Compounds					Ovalue
45) Dimethylphthalate	13.75	163	448757	6.585	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022120\
Data File : BP001830.D
Acq On : 21 Feb 2020 19:03
Operator : CG/JU
Sample : L1506-04
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBCY2

Quant Time: Feb 22 03:46:23 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 22 03:43:48 2020
Response via : Initial Calibration

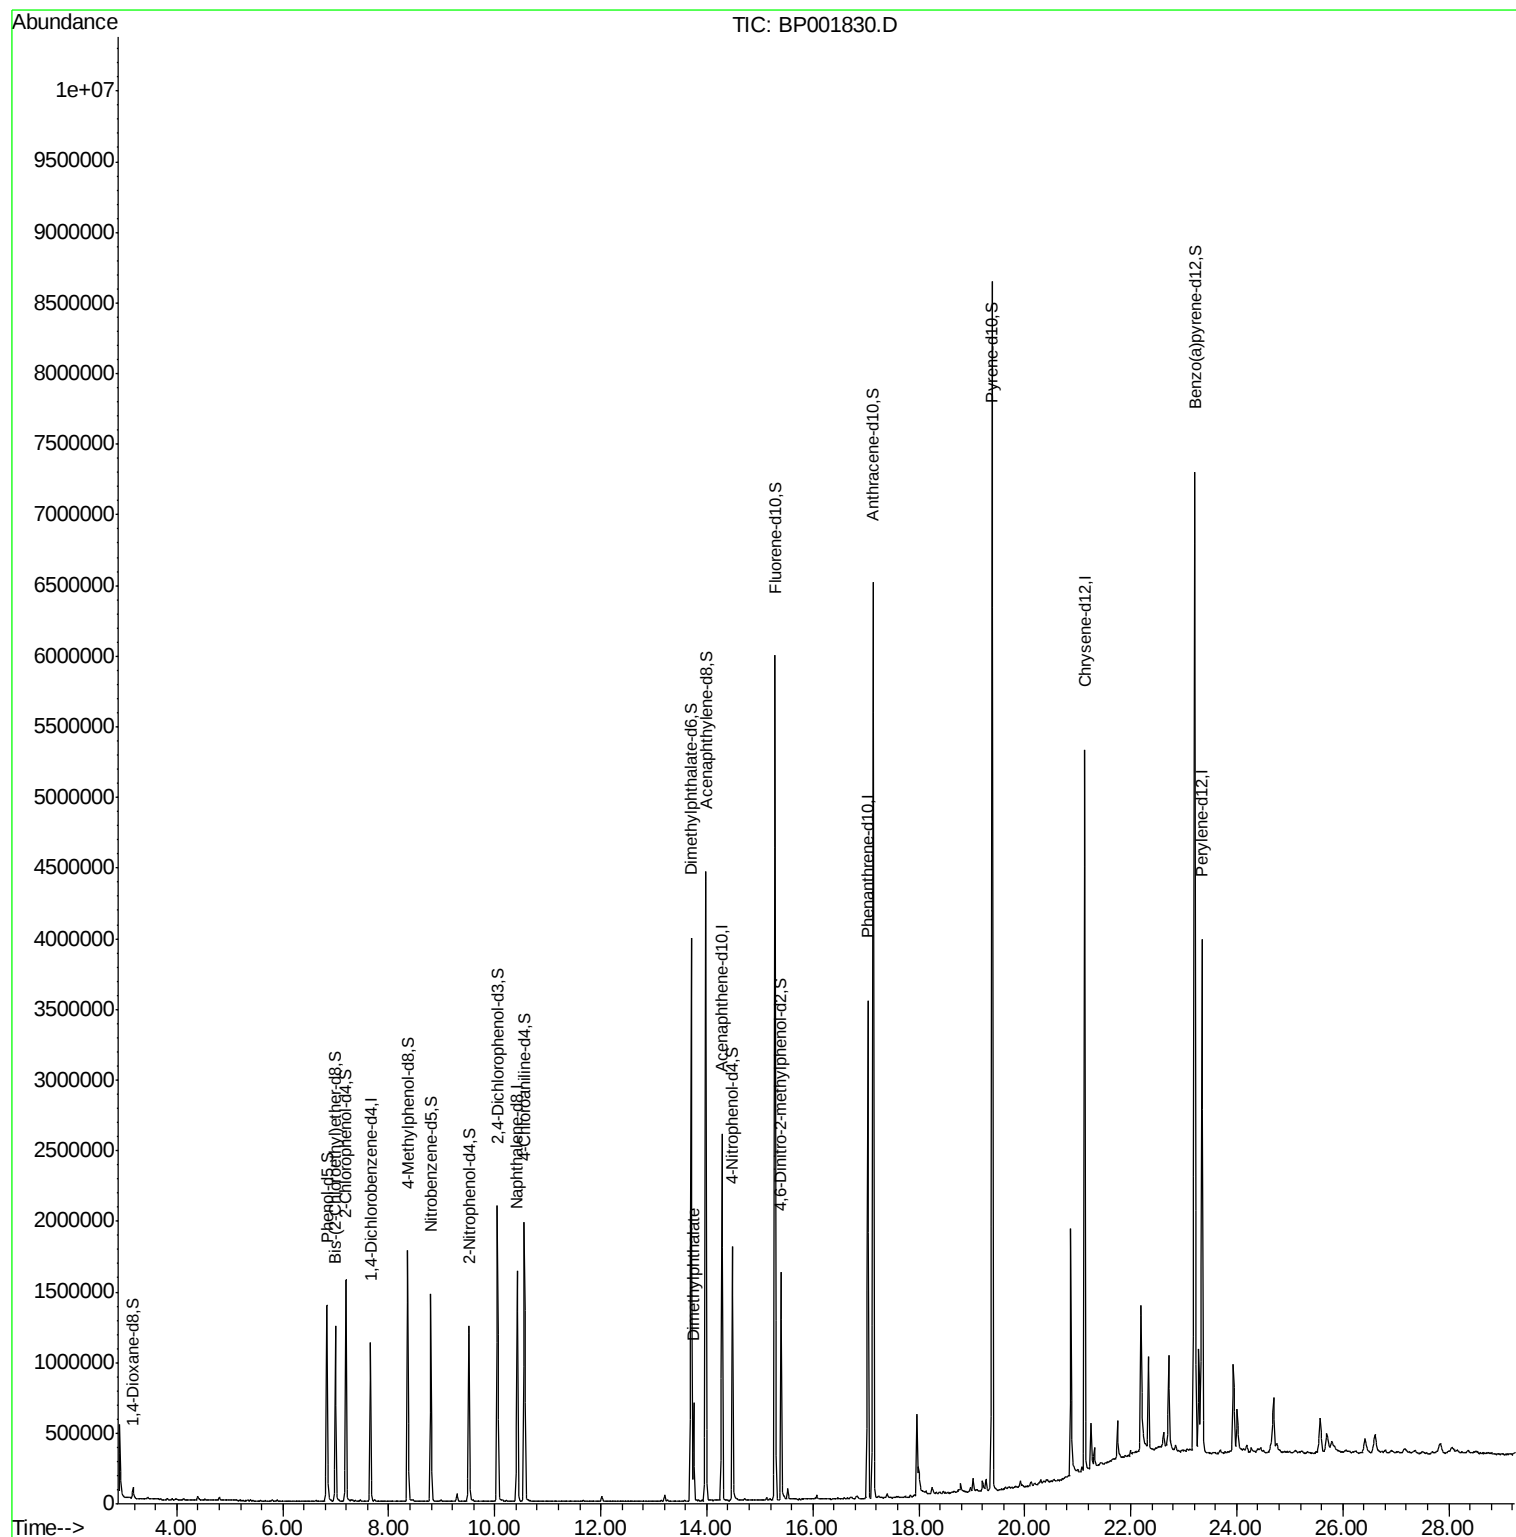

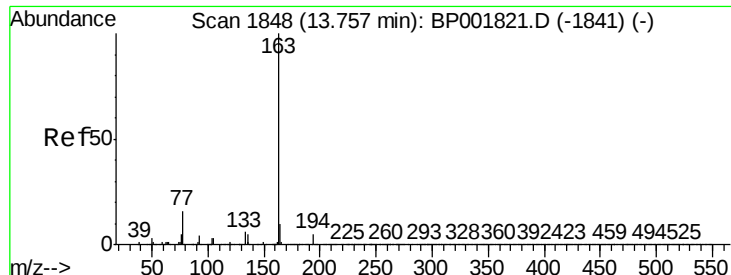

#45

Dimethylphthalate

Concen: 6.585 ng/ul

RT: 13.75 min Scan# 1847

Delta R.T. -0.01 min

Lab File: BP001830.D

Acq: 21 Feb 2020 19:03

Instrument :

BNA_P

ClientSampleId :

DBCY2


Tot Ion:163 Resp: 448757

Ion Ratio Lower Upper

163 100

194 4.1 3.5 5.3

164 9.9 8.0 12.0

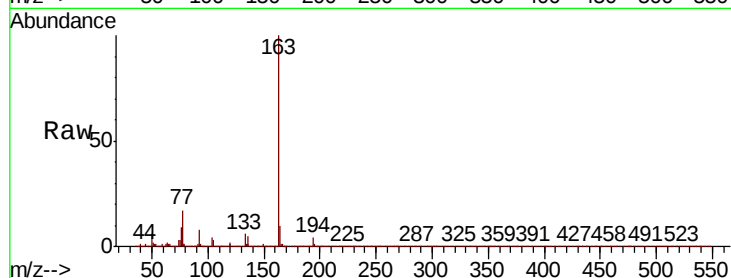

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

