

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022120\
 Data File : BP001831.D
 Acq On : 21 Feb 2020 19:37
 Operator : CG/JU
 Sample : L1506-05
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBCY3

Quant Time: Feb 22 03:46:33 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 22 03:43:48 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	372261	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1608585	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1058504	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2441938	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2540719	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	2931743	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.17	96	48275	5.39	ng/uL	0.00
5) Phenol-d5	6.83	99	955735	33.98	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	559248	34.22	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	852244	37.49	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	818152	36.67	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	430547	39.54	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	488828	49.64	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	885337	37.81	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	1238308	44.71	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	2932577	39.48	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	3460377	37.83	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	501453	38.77	ng/ul	0.00
58) Fluorene-d10	15.29	176	2559612	38.32	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	409693	42.55	ng/ul	0.00
71) Anthracene-d10	17.14	188	3945905	36.68	ng/ul	0.00
79) Pyrene-d10	19.39	212	4670943	35.83	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.20	264	5444208	38.45	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.75	163	373045	4.772	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022120\
Data File : BP001831.D
Acq On : 21 Feb 2020 19:37
Operator : CG/JU
Sample : L1506-05
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBCY3

Quant Time: Feb 22 03:46:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 22 03:43:48 2020
Response via : Initial Calibration

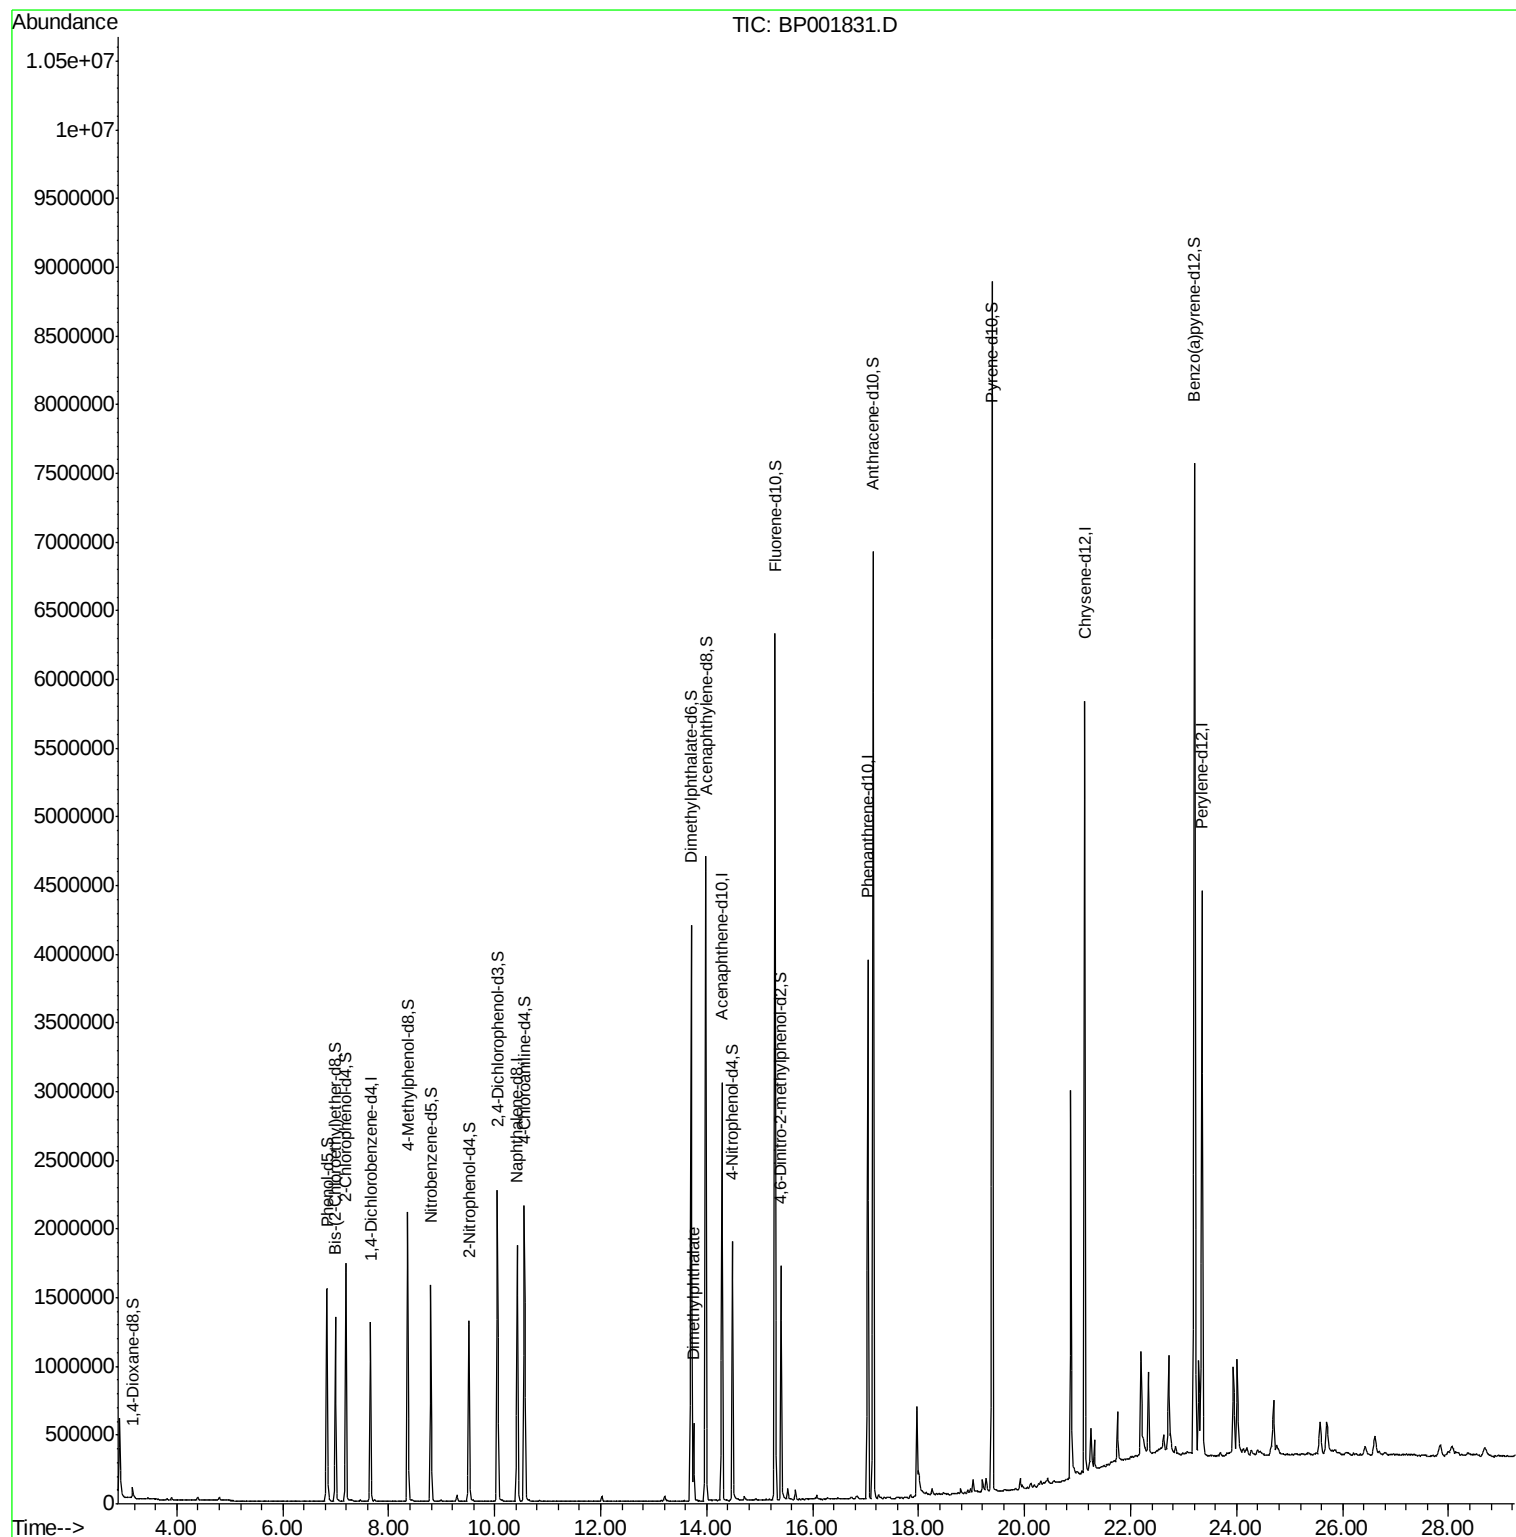

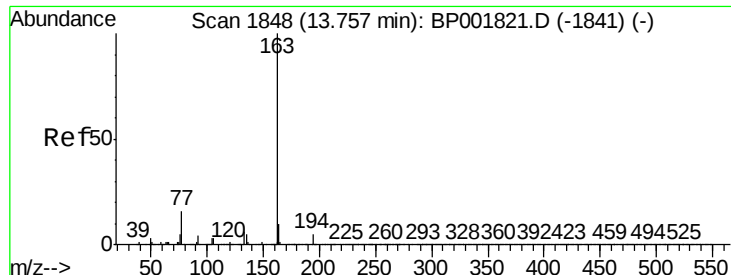

#45

Dimethylphthalate

Concen: 4.772 ng/ul

RT: 13.75 min Scan# 1847

Delta R.T. -0.01 min

Lab File: BP001831.D

Acq: 21 Feb 2020 19:37

Instrument :

BNA_P

ClientSampleId :

DBCY3


Tot Ion:163 Resp: 373045

Ion Ratio Lower Upper

163 100

194 4.4 3.5 5.3

164 9.8 8.0 12.0

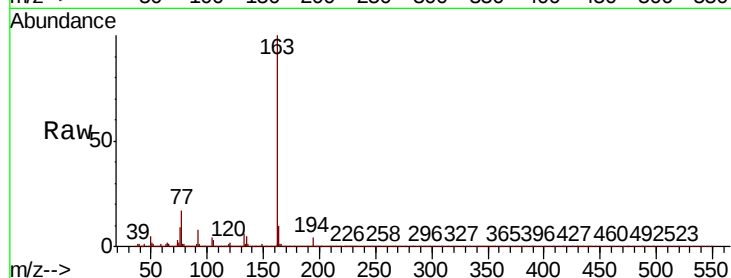

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

