

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022120\
 Data File : BP001837.D
 Acq On : 21 Feb 2020 23:33
 Operator : CG/JU
 Sample : L1506-10
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBCY8

Quant Time: Feb 22 04:18:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 22 04:14:01 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	376590	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1635355	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1065419	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2466171	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2523713	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	2830220	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.18	96	51107	5.64	ng/uL	0.00
5) Phenol-d5	6.83	99	1011241	35.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	568229	34.37	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	877601	38.16	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	852888	37.79	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	442976	40.01	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	498490	49.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	923777	38.80	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	1239295	44.01	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	2909803	38.92	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	3478379	37.78	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	524257	40.27	ng/ul	0.00
58) Fluorene-d10	15.29	176	2589700	38.52	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	393178	40.44	ng/ul	0.00
71) Anthracene-d10	17.14	188	3890687	35.81	ng/ul	0.00
79) Pyrene-d10	19.39	212	4545930	35.10	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	5242877	38.36	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.75	163	402830	5.119	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022120\
Data File : BP001837.D
Acq On : 21 Feb 2020 23:33
Operator : CG/JU
Sample : L1506-10
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBCY8

Quant Time: Feb 22 04:18:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 22 04:14:01 2020
Response via : Initial Calibration

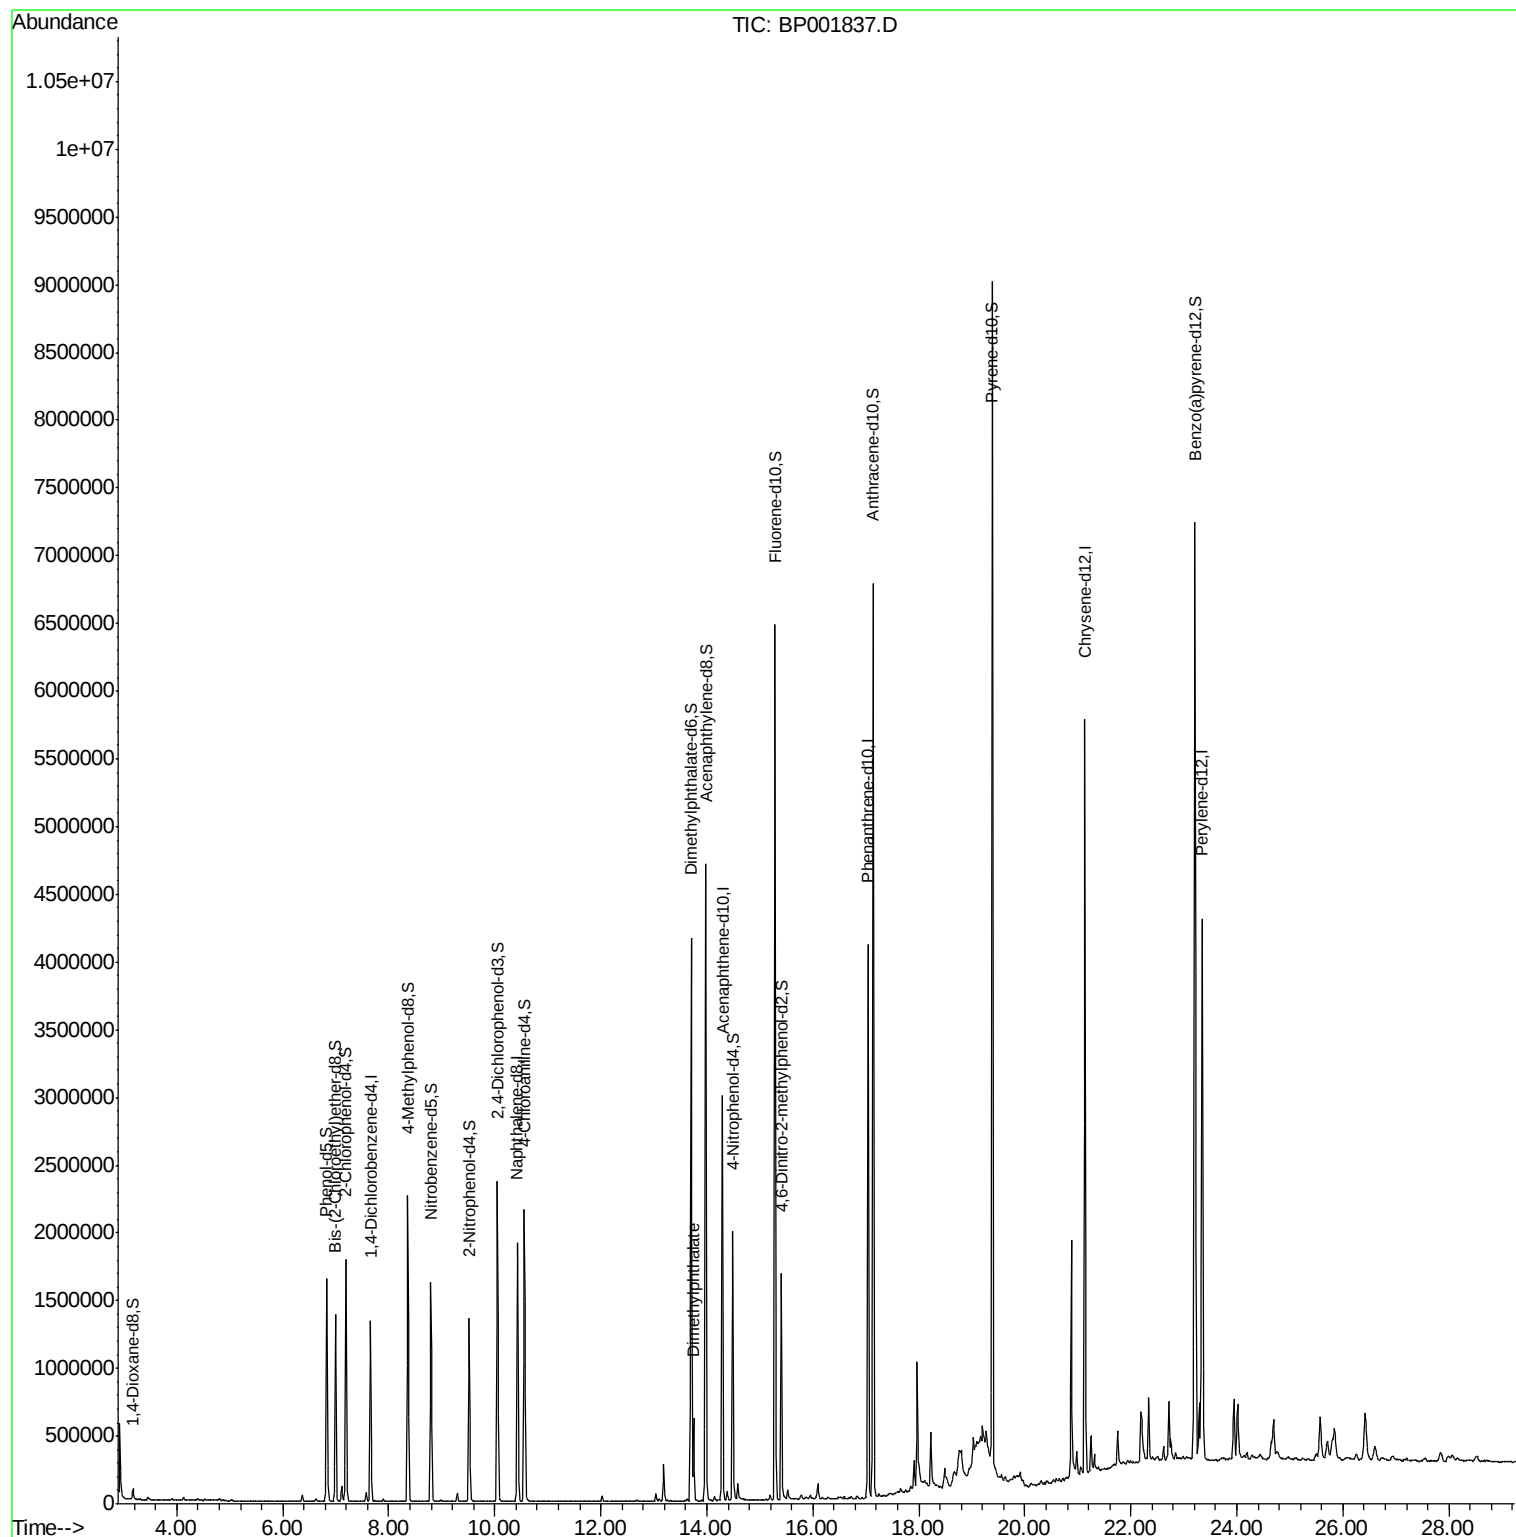

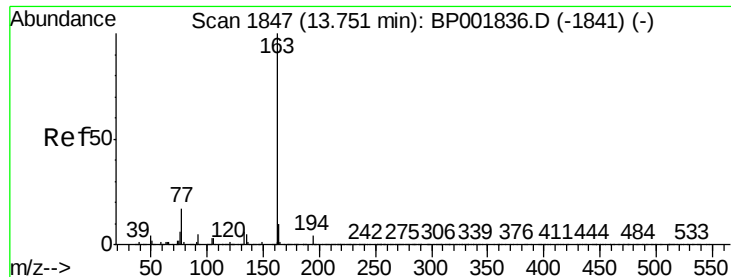

#45

Dimethylphthalate

Concen: 5.119 ng/ul

RT: 13.75 min Scan# 1847

Delta R.T. -0.00 min

Lab File: BP001837.D

Acq: 21 Feb 2020 23:33

Instrument :

BNA_P

ClientSampleId :

DBCY8


Tot Ion:163 Resp: 402830

Ion Ratio Lower Upper

163 100

194 4.3 3.5 5.3

164 9.9 8.0 12.0

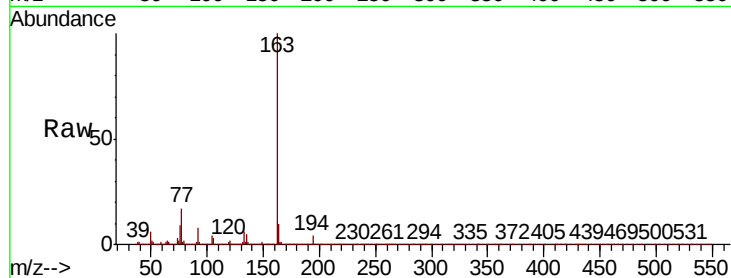

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

