

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022120\
 Data File : BP001840.D
 Acq On : 22 Feb 2020 01:14
 Operator : CG/JU
 Sample : L1506-13
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBCZ1

Quant Time: Feb 22 04:19:04 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 22 04:14:01 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	440000	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1816114	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1146247	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2598781	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2508024	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	2516985	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.18	96	73668	6.95	ng/uL	0.00
5) Phenol-d5	6.83	99	1302017	39.16	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	752856	38.98	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	1168142	43.48	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	1021324	38.73	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	578854	47.08	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	657913	59.17	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	1172556	44.35	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	1571104	50.24	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	3579880	44.50	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	4245421	42.86	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	622612	44.45	ng/ul	0.00
58) Fluorene-d10	15.29	176	3087220	42.68	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	505589	49.35	ng/ul	0.00
71) Anthracene-d10	17.14	188	4705232	41.10	ng/ul	0.00
79) Pyrene-d10	19.39	212	5299835	41.18	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	5327253	43.82	ng/ul	0.00

Target Compounds


				Ovalue	
6) Phenol	6.86	94	54143	1.537	ng/ul 94
45) Dimethylphthalate	13.75	163	457472	5.403	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022120\
Data File : BP001840.D
Acq On : 22 Feb 2020 01:14
Operator : CG/JU
Sample : L1506-13
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBCZ1

Quant Time: Feb 22 04:19:04 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 22 04:14:01 2020
Response via : Initial Calibration

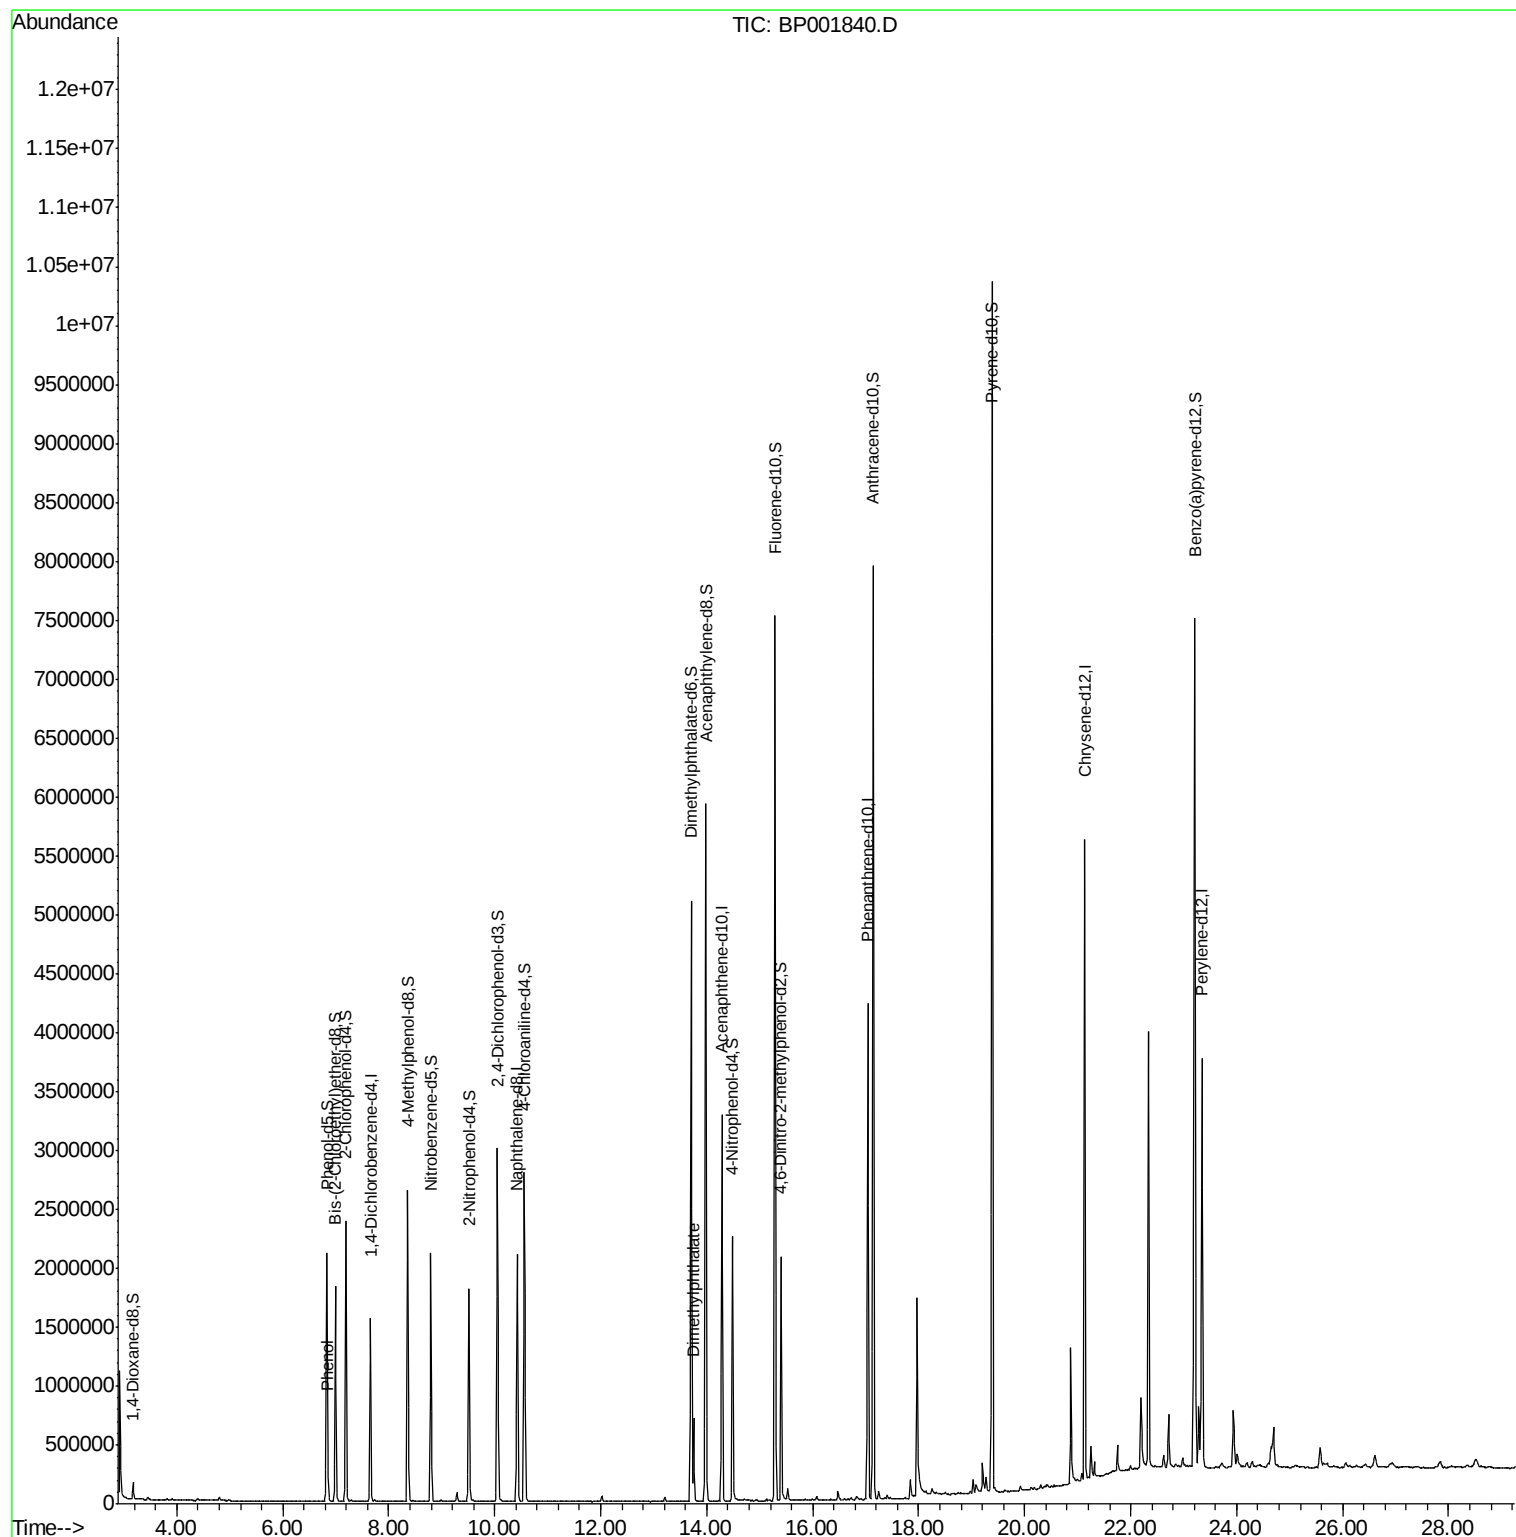

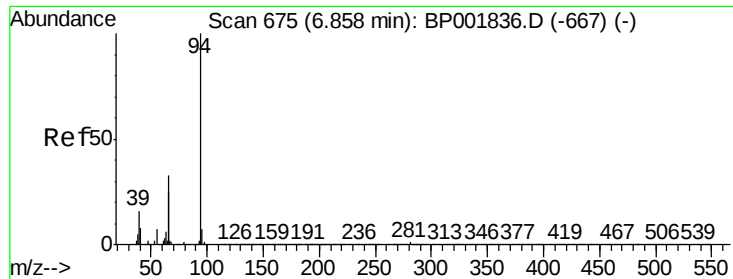

#6

Phenol

Concen: 1.537 ng/ul

RT: 6.86 min Scan# 675

Delta R.T. -0.00 min

Lab File: BP001840.D

Acq: 22 Feb 2020 01:14

Instrument :

BNA_P

ClientSampleId :

DBCZ1





Tot Ion: 94 Resp: 54143

Ion Ratio Lower Upper

94 100

65 26.7 19.8 29.6

66 37.9 26.6 39.8

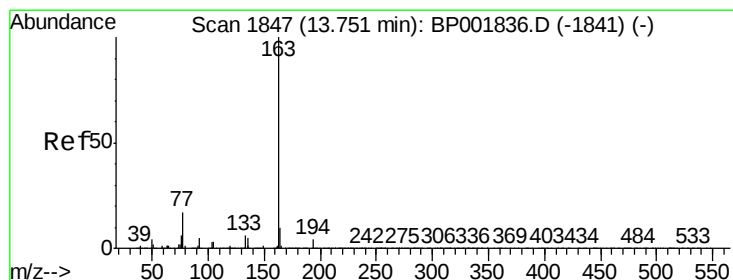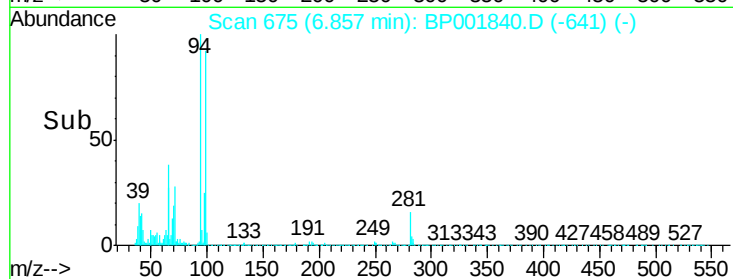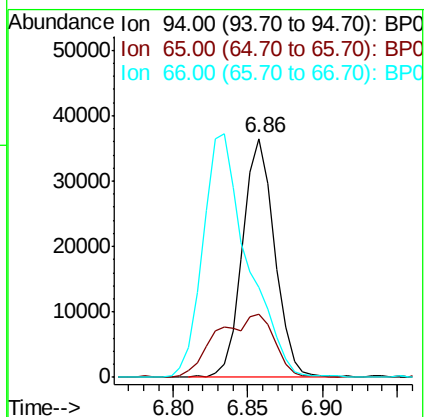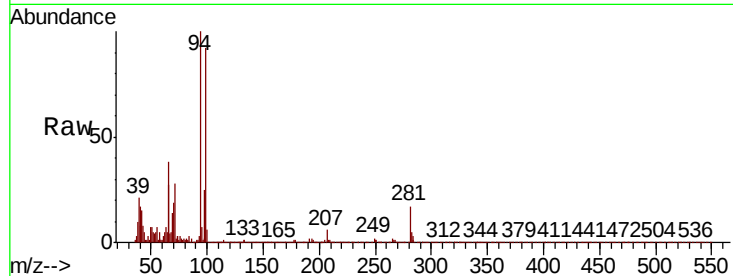

#45

Dimethylphthalate

Concen: 5.403 ng/ul

RT: 13.75 min Scan# 1847

Delta R.T. -0.00 min

Lab File: BP001840.D

Acq: 22 Feb 2020 01:14

Tgt Ion: 163 Resp: 457472

Ion Ratio Lower Upper

163 100

194 4.3 3.5 5.3

164 9.9 8.0 12.0

