

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022120\
 Data File : BP001843.D
 Acq On : 22 Feb 2020 02:55
 Operator : CG/JU
 Sample : L1506-16
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBCZ4

Quant Time: Feb 22 04:19:34 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Feb 22 04:14:01 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	420582	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1795010	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1152240	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2635172	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2647470	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	2859617	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.18	96	62184	6.14	ng/uL	0.00
5) Phenol-d5	6.83	99	1247681	39.26	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	698913	37.85	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	1085711	42.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	1073725	42.60	ng/ul	0.00
19) Nitrobenzene-d5	8.80	128	554367	45.62	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	636878	57.96	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	1142913	43.74	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	1577257	51.03	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	3604169	44.57	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	4246348	42.65	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	681152	48.38	ng/ul	0.00
58) Fluorene-d10	15.29	176	3115519	42.84	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	543683	52.33	ng/ul	0.00
71) Anthracene-d10	17.14	188	4749823	40.92	ng/ul	0.00
79) Pyrene-d10	19.39	212	5442799	40.06	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	6079759	44.02	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
45) Dimethylphthalate	13.75	163	499533	5.870	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022120\
Data File : BP001843.D
Acq On : 22 Feb 2020 02:55
Operator : CG/JU
Sample : L1506-16
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBCZ4

Quant Time: Feb 22 04:19:34 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Feb 22 04:14:01 2020
Response via : Initial Calibration

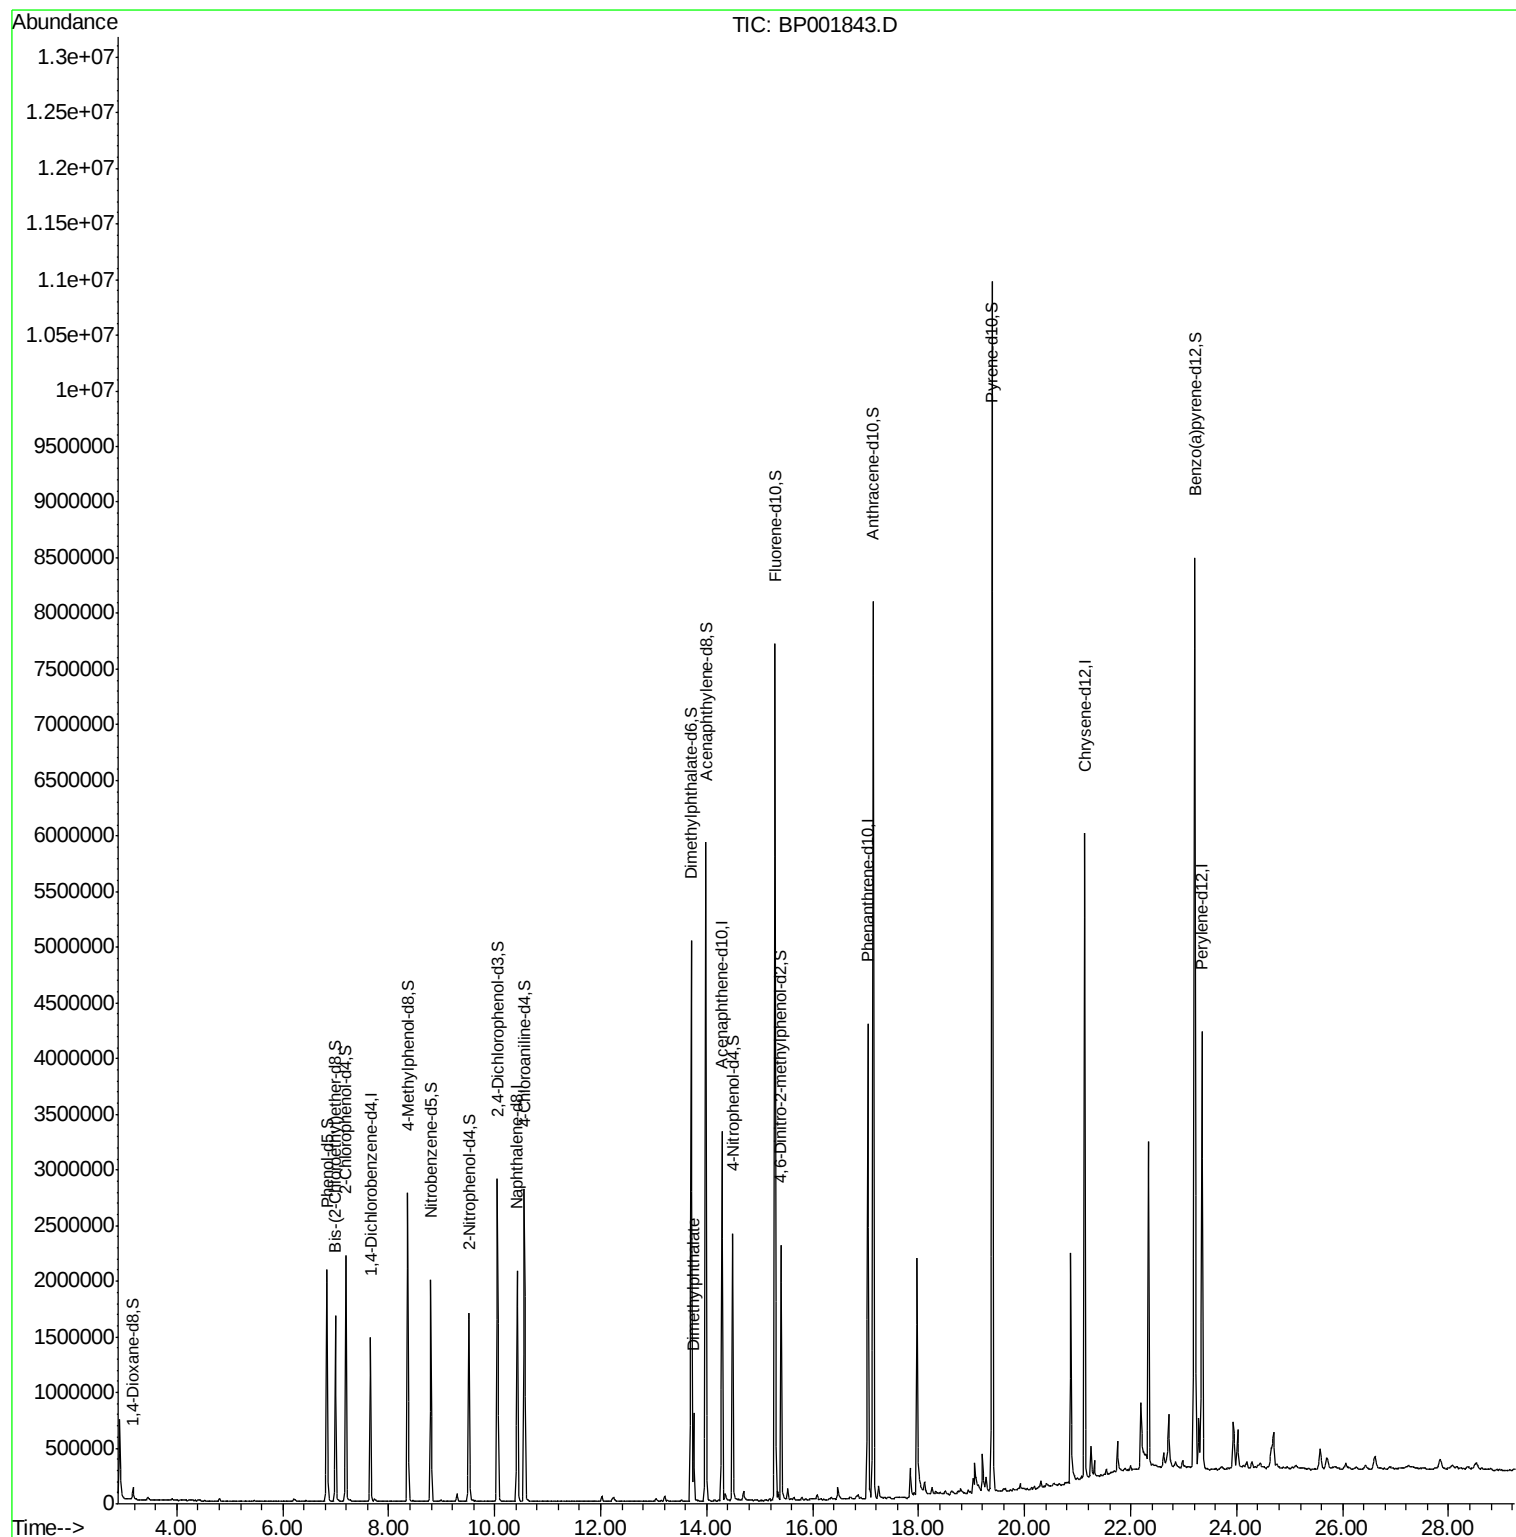

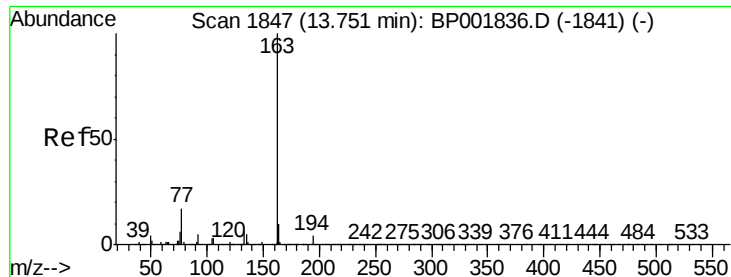

#45

Dimethylphthalate

Concen: 5.870 ng/ul

RT: 13.75 min Scan# 1847

Delta R.T. -0.00 min

Lab File: BP001843.D

Acq: 22 Feb 2020 02:55

Instrument :

BNA_P

ClientSampleId :

DBCZ4


Tot Ion:163 Resp: 499533

Ion Ratio Lower Upper

163 100

194 4.5 3.5 5.3

164 10.3 8.0 12.0

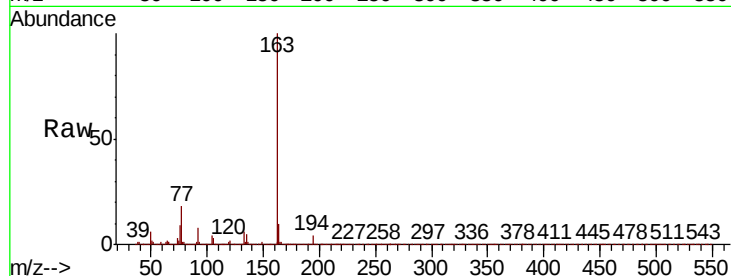

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

