

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022120\
 Data File : BP001846.D
 Acq On : 22 Feb 2020 04:36
 Operator : CG/JU
 Sample : L1506-19
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBCZ7

Quant Time: Feb 24 01:19:46 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 24 01:10:13 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	366313	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1585967	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1037853	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2391385	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2478050	20.00	ng/ul	0.00
86) Perylene-d12	23.34	264	2773013	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.18	96	38869	4.41	ng/uL	0.00
5) Phenol-d5	6.83	99	736492	26.61	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	432087	26.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	647013	28.93	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	637704	29.05	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	335728	31.27	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	354539	36.52	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	666673	28.88	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	761977	27.90	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	2253972	30.95	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	2743152	30.59	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	315302	24.86	ng/ul	0.00
58) Fluorene-d10	15.29	176	2048403	31.27	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	239639	25.42	ng/ul	0.00
71) Anthracene-d10	17.14	188	3219422	30.56	ng/ul	0.00
79) Pyrene-d10	19.39	212	3796774	29.86	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	4343573	32.43	ng/ul	0.00


Target Compounds					Ovalue	
45) Dimethylphthalate	13.75	163	239896	3.129	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022120\
Data File : BP001846.D
Acq On : 22 Feb 2020 04:36
Operator : CG/JU
Sample : L1506-19
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBCZ7

Quant Time: Feb 24 01:19:46 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 01:10:13 2020
Response via : Initial Calibration

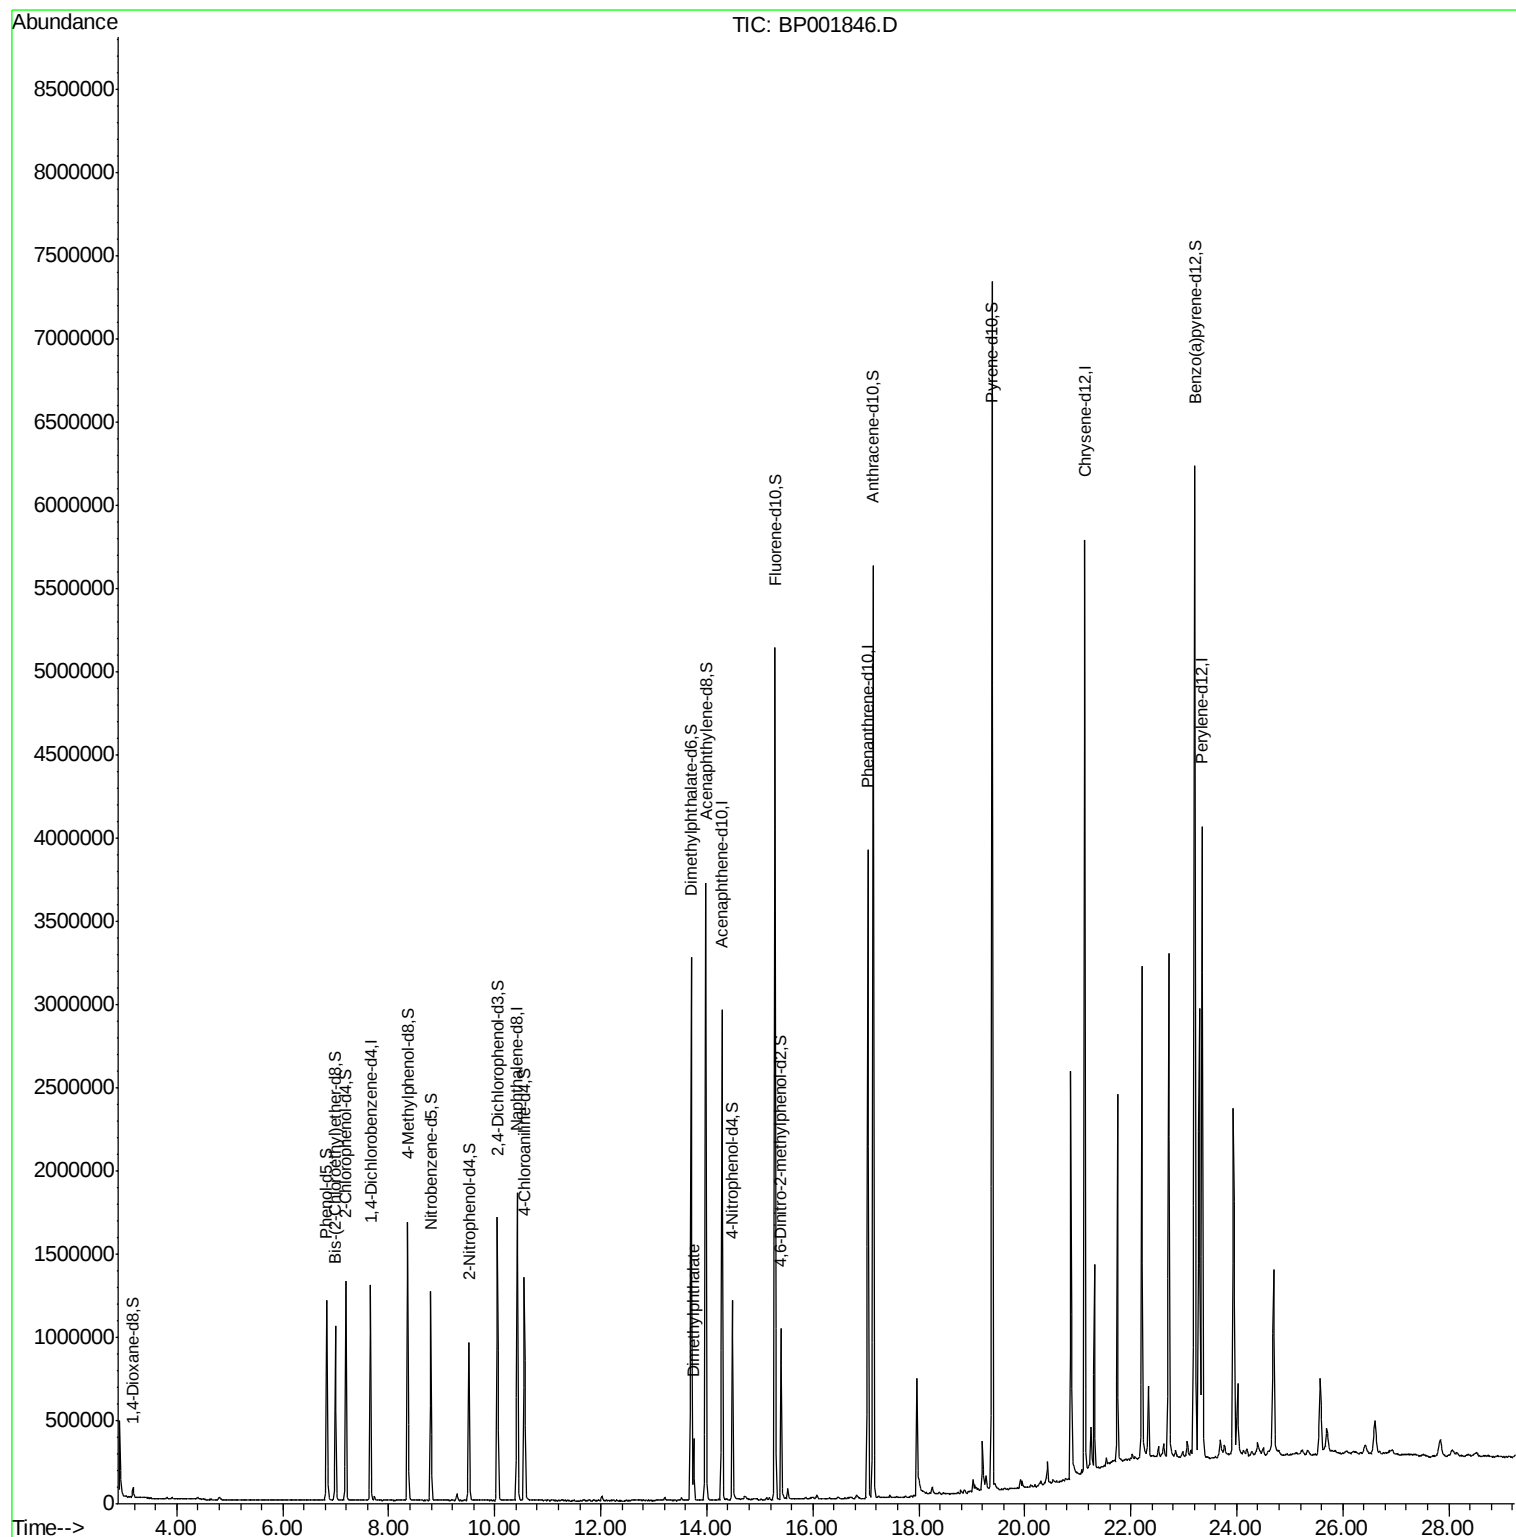

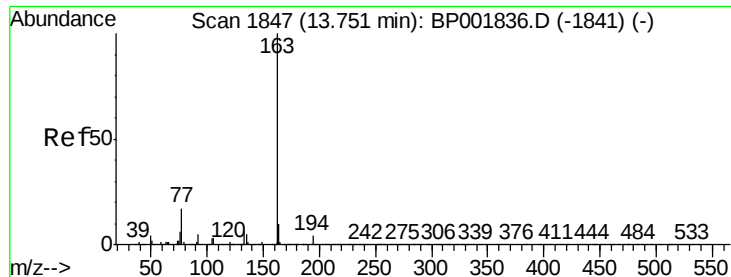

#45

Dimethylphthalate

Concen: 3.129 ng/ul

RT: 13.75 min Scan# 1847

Delta R.T. -0.00 min

Lab File: BP001846.D

Acq: 22 Feb 2020 04:36

Instrument :

BNA_P

ClientSampleId :

DBCZ7


Tot Ion:163 Resp: 239896

Ion Ratio Lower Upper

163 100

194 4.3 3.5 5.3

164 9.7 8.0 12.0

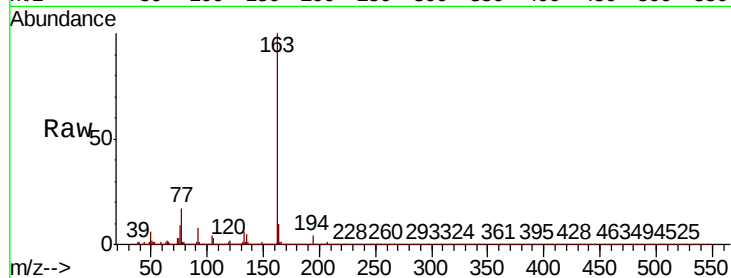

Abundance Ion 163.00 (162.70 to 163.70): E

250000 Ion 194.00 (193.70 to 194.70): E

200000 Ion 164.00 (163.70 to 164.70): E

