

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP022120\
 Data File : BP001848.D
 Acq On : 22 Feb 2020 05:44
 Operator : CG/JU
 Sample : L1506-21
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBCZ9

Quant Time: Feb 24 01:13:13 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Feb 24 01:10:13 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.65	152	371240	20.00	ng/ul	0.00
18) Naphthalene-d8	10.43	136	1575864	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.29	164	1029553	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.04	188	2358616	20.00	ng/ul	0.00
78) Chrysene-d12	21.13	240	2446411	20.00	ng/ul	0.00
86) Perylene-d12	23.35	264	2745909	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.18	96	49971	5.59	ng/uL	0.00
5) Phenol-d5	6.83	99	1040428	37.09	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.99	67	588449	36.11	ng/ul	0.00
9) 2-Chlorophenol-d4	7.19	132	906942	40.01	ng/ul	0.00
13) 4-Methylphenol-d8	8.36	113	904851	40.67	ng/ul	0.00
19) Nitrobenzene-d5	8.79	128	473062	44.34	ng/ul	0.00
22) 2-Nitrophenol-d4	9.52	143	539746	55.95	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.05	165	968362	42.21	ng/ul	0.00
29) 4-Chloroaniline-d4	10.56	131	1356704	50.00	ng/ul	0.00
44) Dimethylphthalate-d6	13.70	166	3140256	43.46	ng/ul	0.00
47) Acenaphthylene-d8	13.98	160	3728711	41.91	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	559500	44.47	ng/ul	0.00
58) Fluorene-d10	15.29	176	2750249	42.33	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.40	200	439721	47.29	ng/ul	0.00
71) Anthracene-d10	17.14	188	4229890	40.71	ng/ul	0.00
79) Pyrene-d10	19.39	212	4917296	39.17	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.21	264	5724276	43.16	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	13.75	163	357417	4.700	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP022120\
Data File : BP001848.D
Acq On : 22 Feb 2020 05:44
Operator : CG/JU
Sample : L1506-21
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBCZ9

Quant Time: Feb 24 01:13:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP021820MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Feb 24 01:10:13 2020
Response via : Initial Calibration

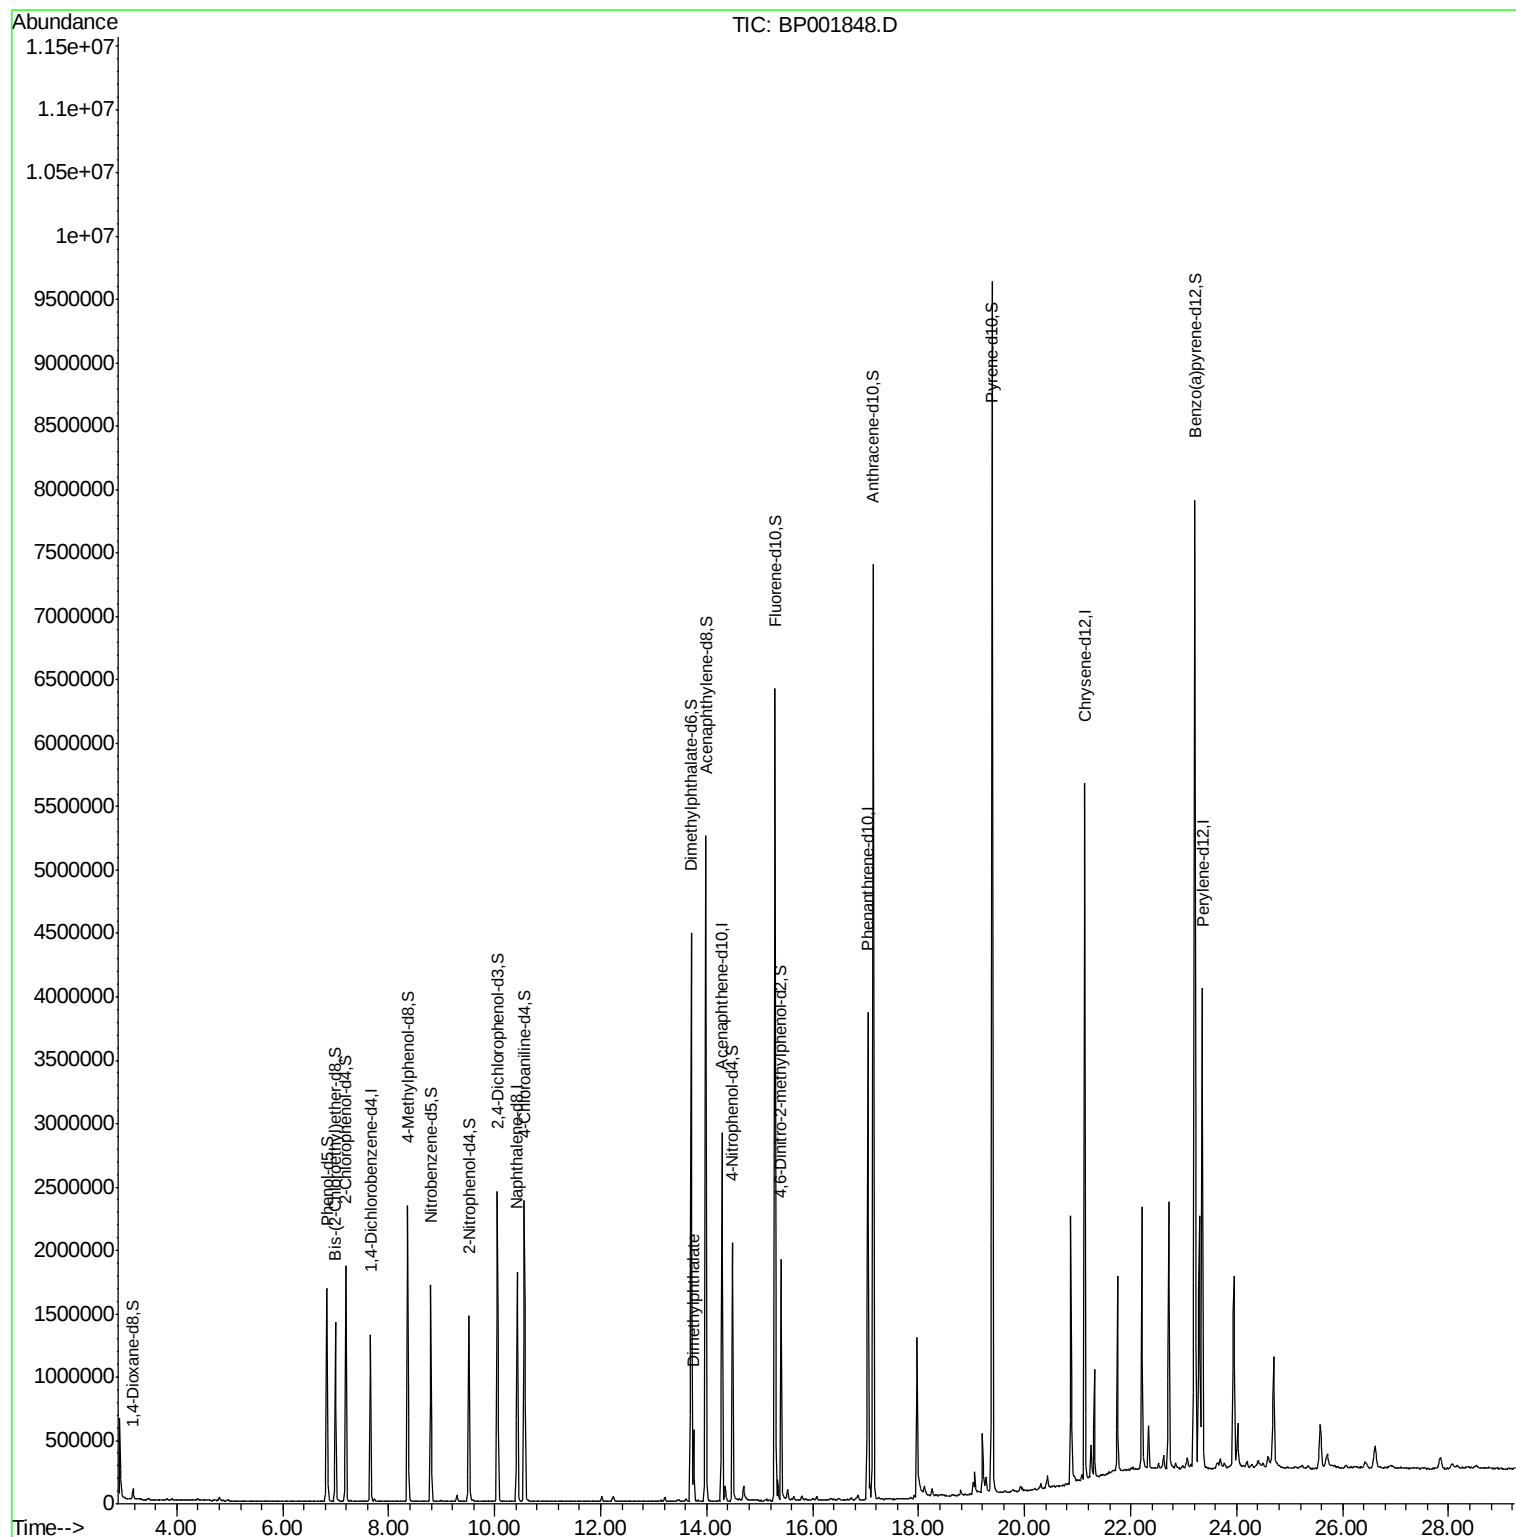

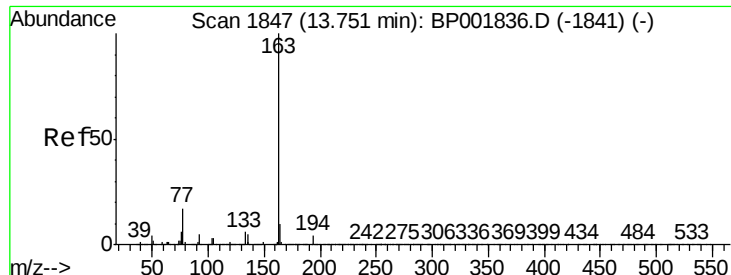

#45

Dimethylphthalate

Concen: 4.700 ng/ul

RT: 13.75 min Scan# 1847

Delta R.T. -0.00 min

Lab File: BP001848.D

Acq: 22 Feb 2020 05:44

Instrument :

BNA_P

ClientSampleId :

DBCZ9


Tot Ion:163 Resp: 357417

Ion Ratio Lower Upper

163 100

194 4.3 3.5 5.3

164 10.1 8.0 12.0

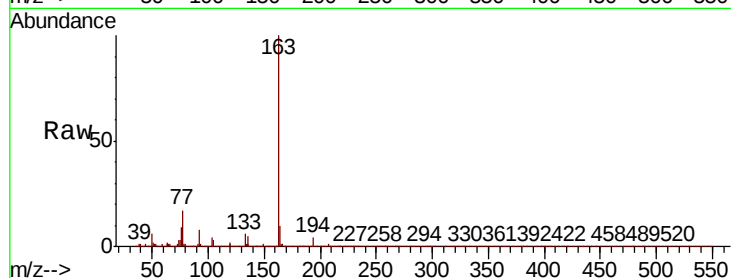

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

