
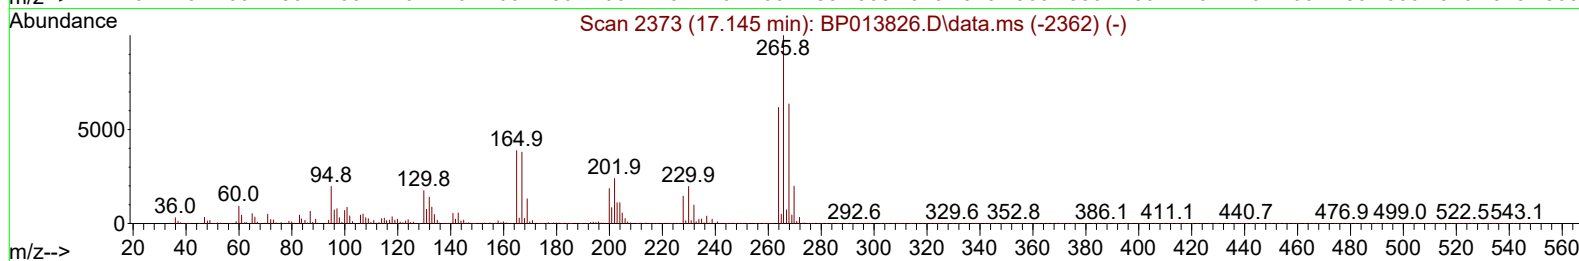
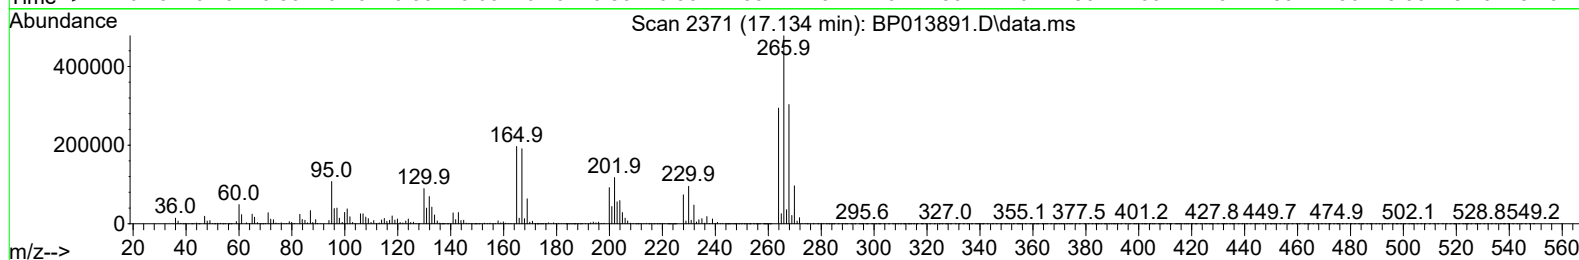


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022823\
 Data File : BP013891.D
 Acq On : 28 Feb 2023 16:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 04:33:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 24 16:57:00 2023
 Response via : Initial Calibration

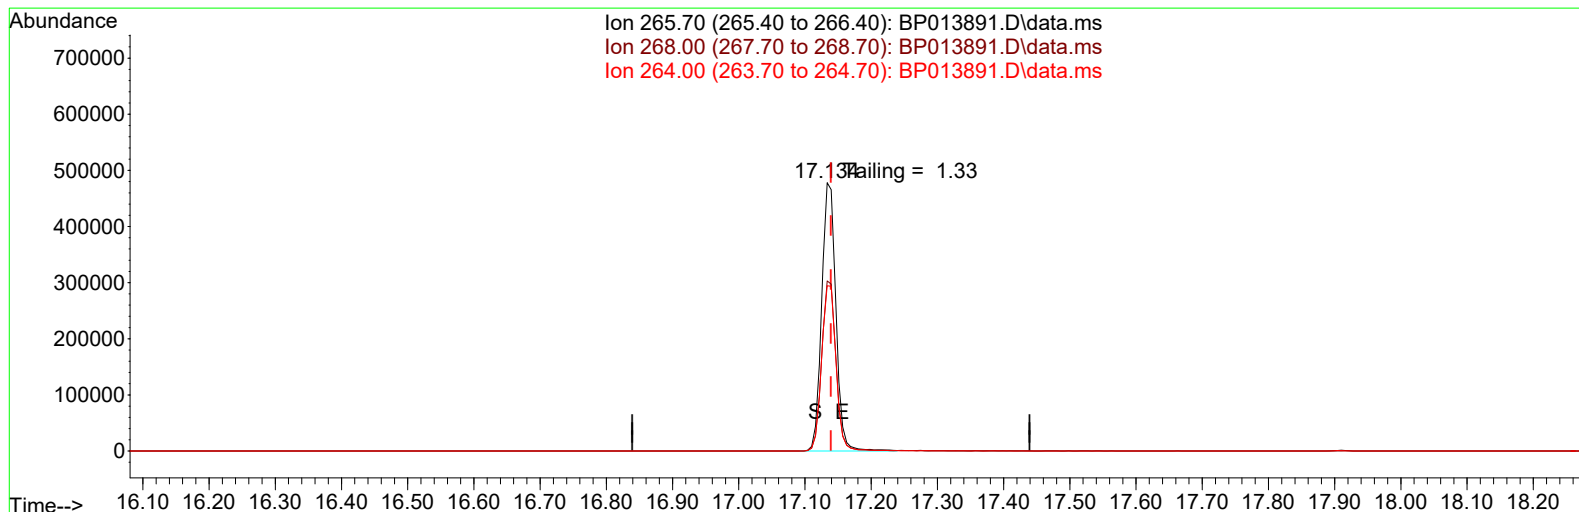

TIC: BP013891.D\data.ms

(70) Pentachlorophenol (C)




17.134min (-0.006) 505435.02 ng

response 710577

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.38
264.00	61.70	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022823\
 Data File : BP013891.D
 Acq On : 28 Feb 2023 16:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 01 04:33:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 24 16:57:00 2023
 Response via : Initial Calibration

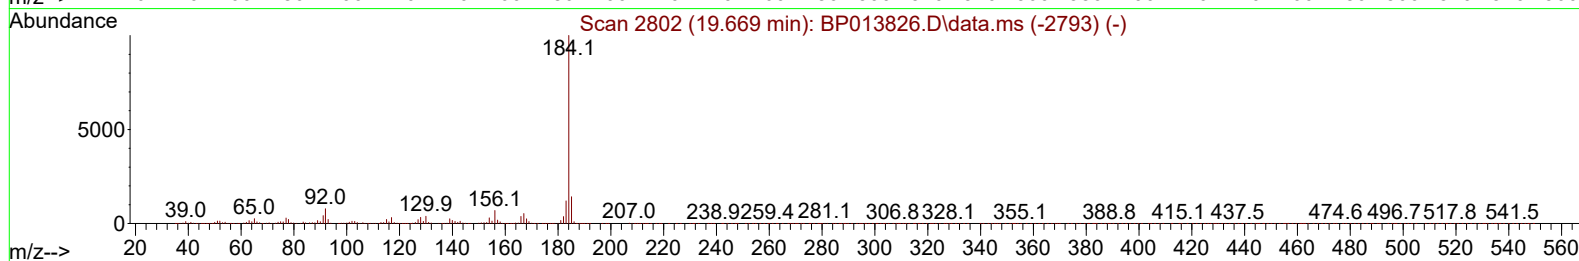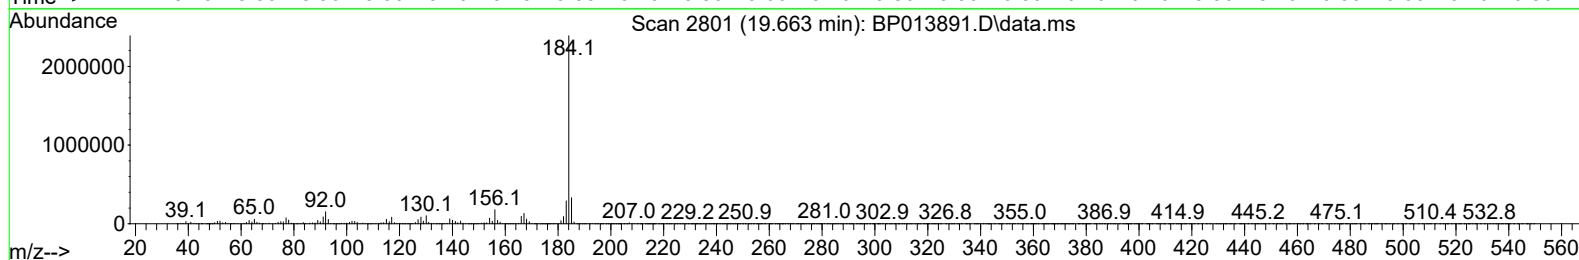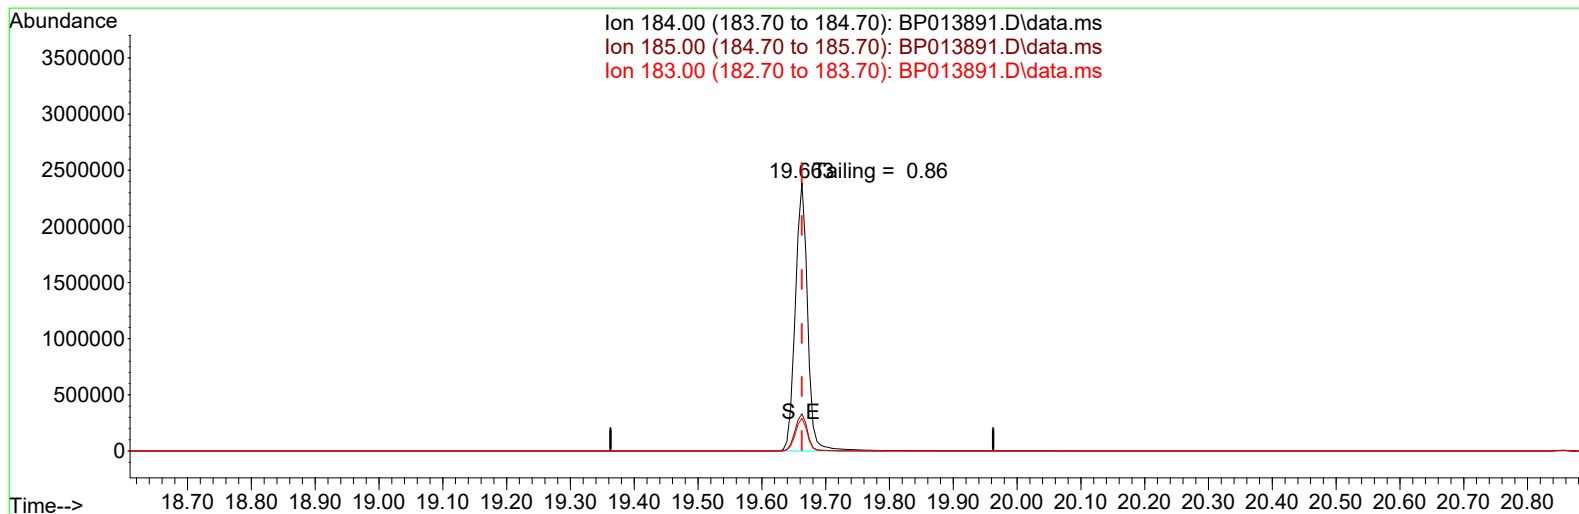

TIC: BP013891.D\data.ms

(77) Benzidine**19.663min (+ 0.000) 138977.71 ng****response 3199622**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.90
183.00	12.00	12.18
0.00	0.00	0.00