

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022823\
 Data File : BP013907.D
 Acq On : 01 Mar 2023 01:10
 Operator : CG/JU
 Sample : 01723-15
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 HH-CON-8

Quant Time: Mar 01 03:51:53 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 24 16:57:00 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.093	152	114301	20.000	ng	-0.01
21) Naphthalene-d8	10.922	136	448908	20.000	ng	0.00
39) Acenaphthene-d10	14.734	164	304192	20.000	ng	0.00
64) Phenanthrene-d10	17.487	188	713869	20.000	ng	0.00
76) Chrysene-d12	21.563	240	695292	20.000	ng	-0.01
86) Perylene-d12	24.110	264	803583	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.634	112	472212	68.088	ng	0.00
7) Phenol-d6	7.246	99	866250	97.526	ng	0.00
23) Nitrobenzene-d5	9.269	82	612988	73.737	ng	-0.01
42) 2,4,6-Tribromophenol	16.222	330	279006	63.009	ng	-0.01
45) 2-Fluorobiphenyl	13.357	172	1518390	65.562	ng	-0.01
79) Terphenyl-d14	20.022	244	2756080	76.265	ng	0.00


Target Compounds Qvalue


 (#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022823\
Data File : BP013907.D
Acq On : 01 Mar 2023 01:10
Operator : CG/JU
Sample : 01723-15
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
HH-CON-8

Quant Time: Mar 01 03:51:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 16:57:00 2023
Response via : Initial Calibration




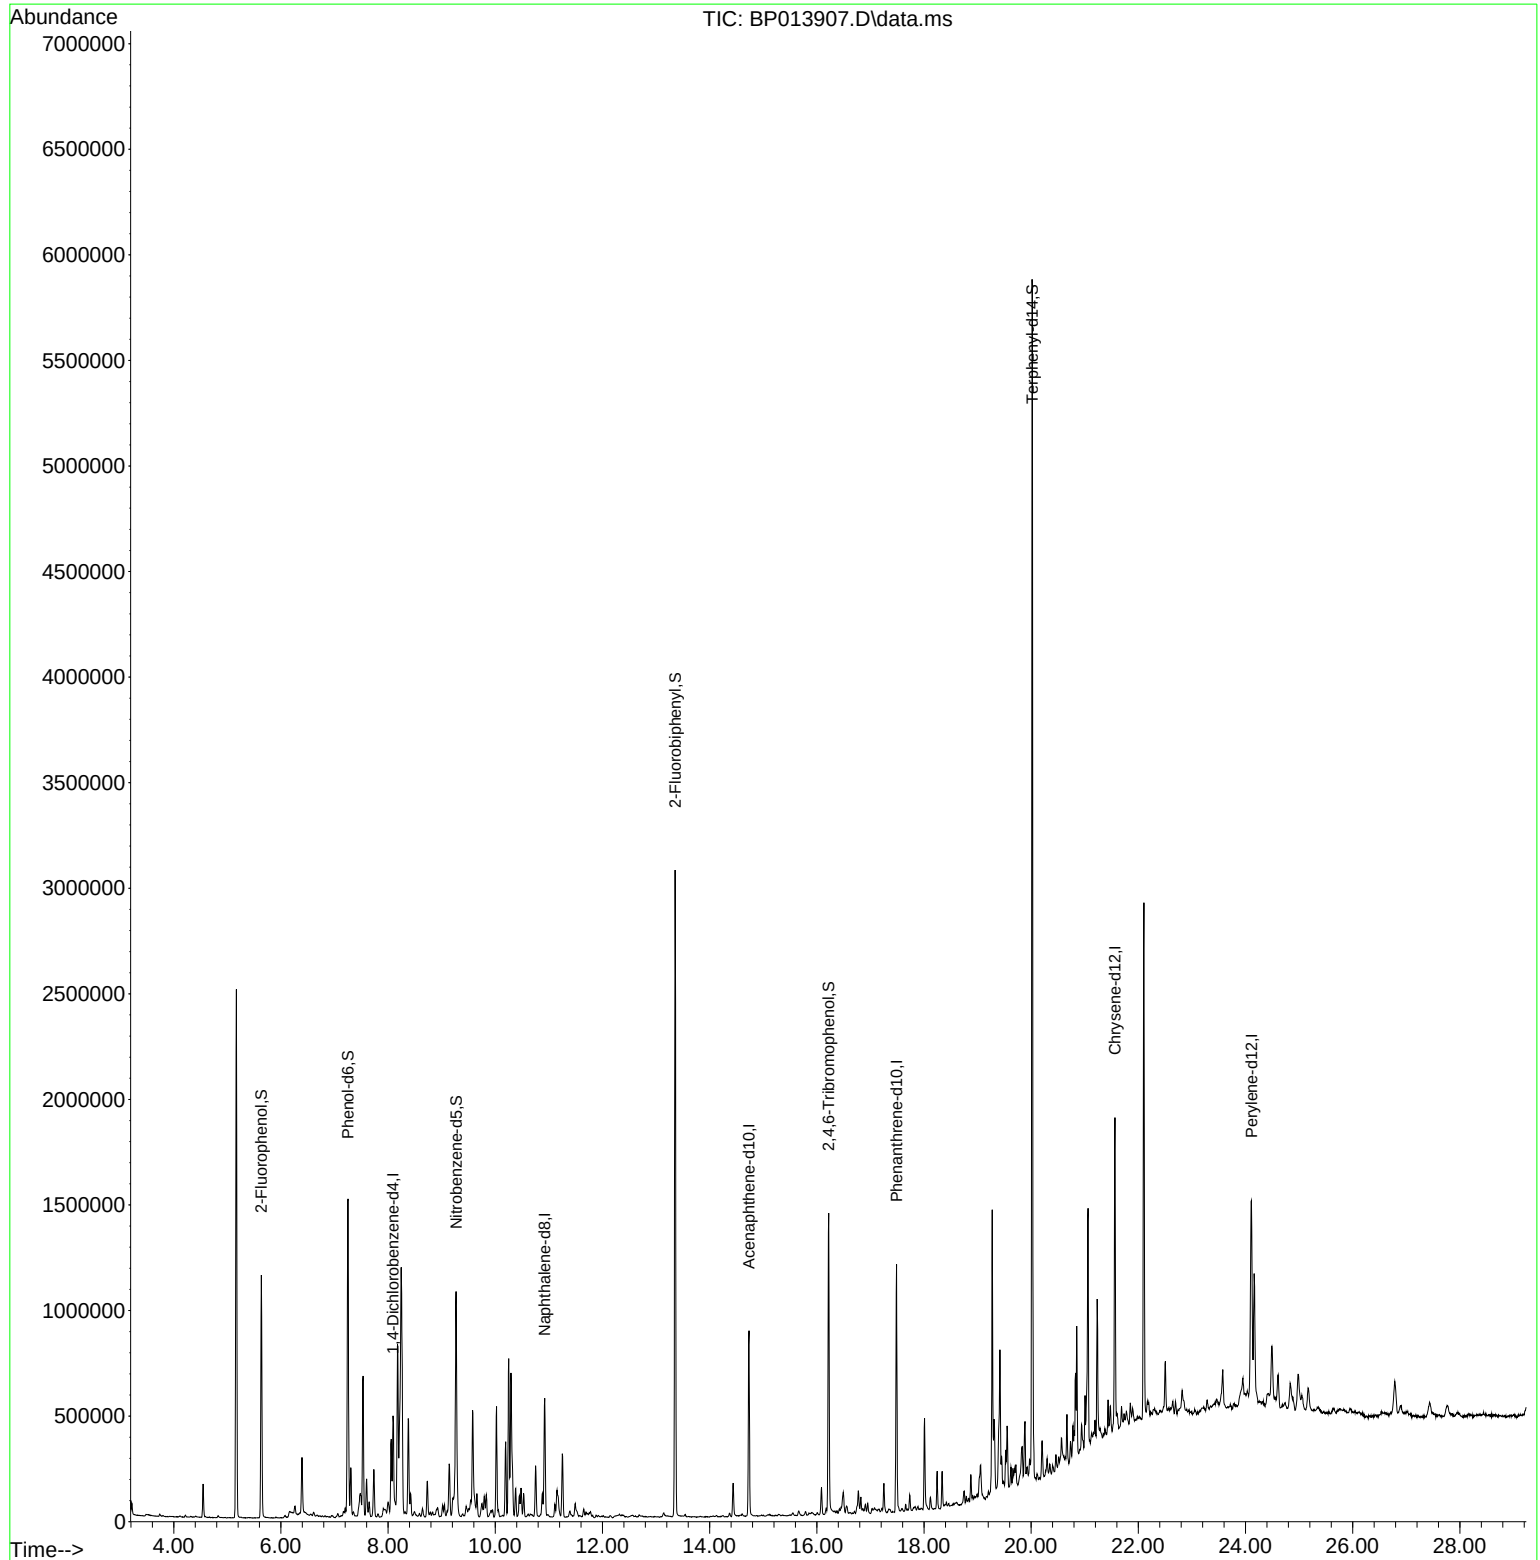




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 8.093 min Scan# 81
Delta R.T. -0.011 min
Lab File: BP013907.D
Acq: 01 Mar 2023 01:10




Instrument :
BNA_P
ClientSampleId :
HH-CON-8


Tgt Ion:152 Resp: 114301
Ion Ratio Lower Upper
152 100
150 155.9 122.8 184.2
115 61.6 49.0 73.6

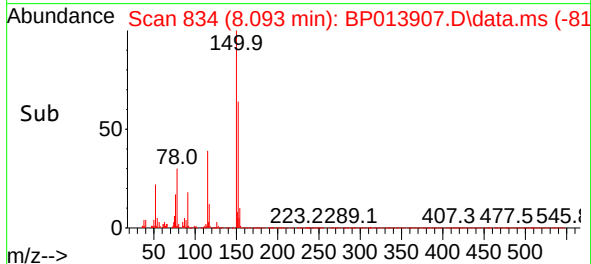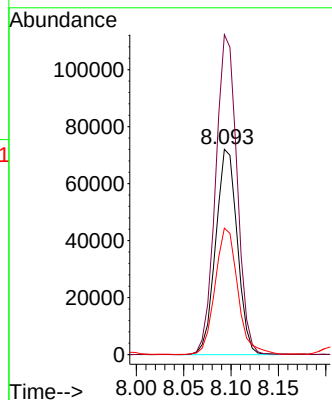

#5
2-Fluorophenol
Concen: 68.088 ng
RT: 5.634 min Scan# 416
Delta R.T. -0.006 min
Lab File: BP013907.D
Acq: 01 Mar 2023 01:10

Tgt Ion:112 Resp: 472212
Ion Ratio Lower Upper
112 100
64 57.5 44.6 66.8
63 32.3 23.6 35.4


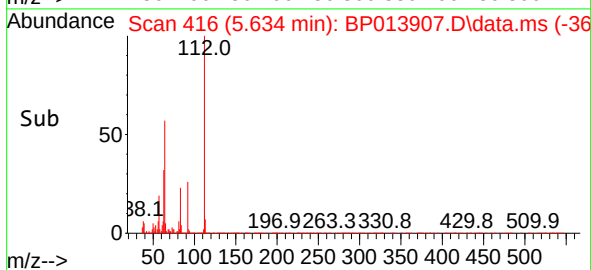
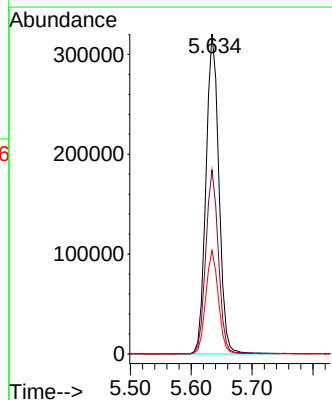
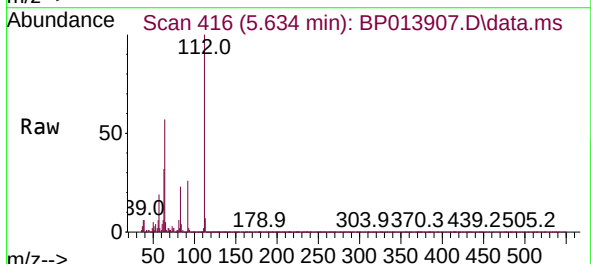




#7
Phenol-d6
Concen: 97.526 ng
RT: 7.246 min Scan# 69
Delta R.T. -0.006 min
Lab File: BP013907.D
Acq: 01 Mar 2023 01:10




Instrument :
BNA_P
ClientSampleId :
HH-CON-8


Tgt Ion:	99	Resp:	866250
Ion	Ratio	Lower	Upper
99	100		
42	17.9	12.5	18.7
71	40.5	27.8	41.8

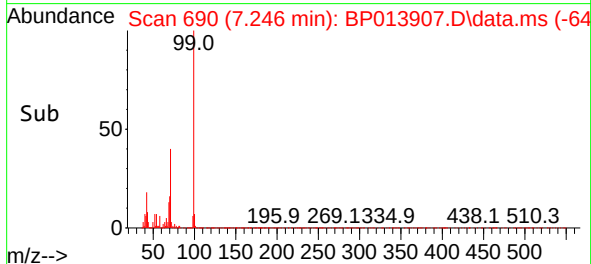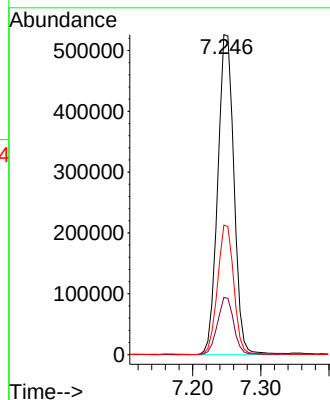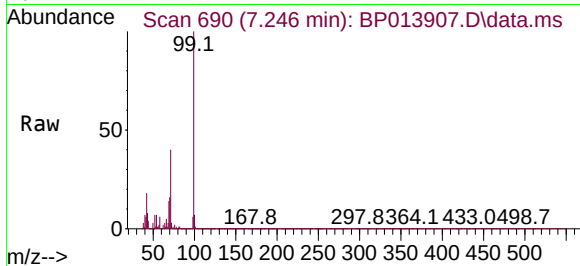

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.922 min Scan# 1315
Delta R.T. -0.006 min
Lab File: BP013907.D
Acq: 01 Mar 2023 01:10

Tgt Ion:	136	Resp:	448908
Ion	Ratio	Lower	Upper
136	100		
137	11.4	8.5	12.7
54	6.7	5.8	8.6
68	5.0	4.6	6.8


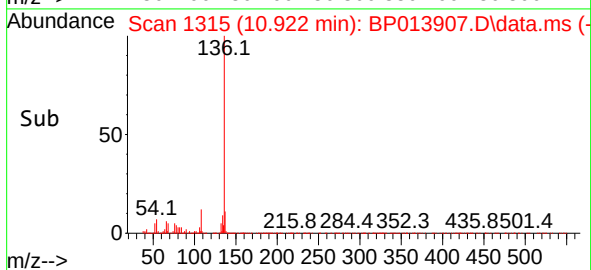
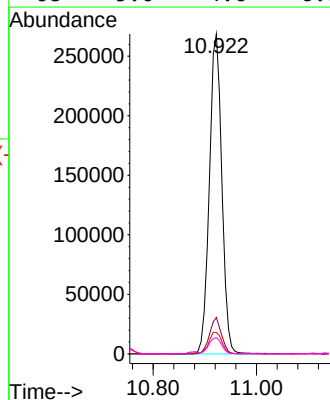
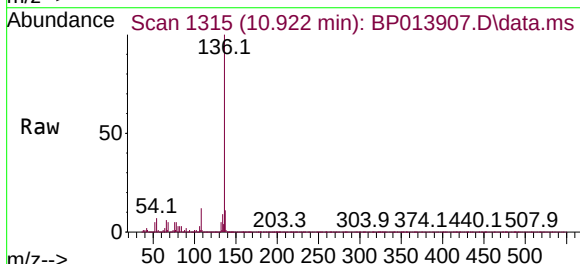




#23
Nitrobenzene-d5
Concen: 73.737 ng
RT: 9.269 min Scan# 1034
Delta R.T. -0.012 min
Lab File: BP013907.D
Acq: 01 Mar 2023 01:10




Instrument :
BNA_P
ClientSampleId :
HH-CON-8


Tgt Ion: 82 Resp: 612988
Ion Ratio Lower Upper
82 100
128 40.6 32.9 49.3
54 46.7 35.6 53.4

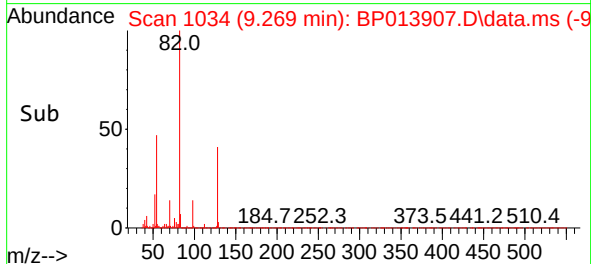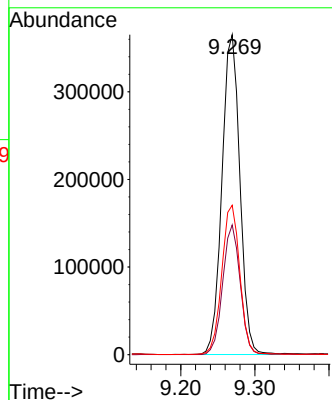

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.734 min Scan# 1963
Delta R.T. -0.006 min
Lab File: BP013907.D
Acq: 01 Mar 2023 01:10

Tgt Ion: 164 Resp: 304192
Ion Ratio Lower Upper
164 100
162 100.4 81.7 122.5
160 44.2 36.1 54.1

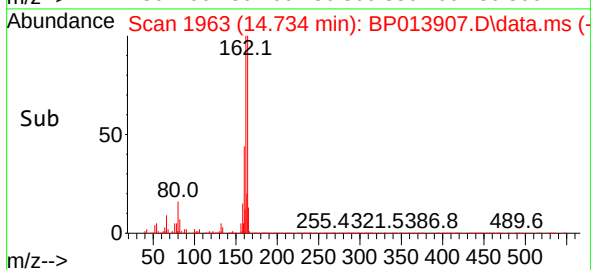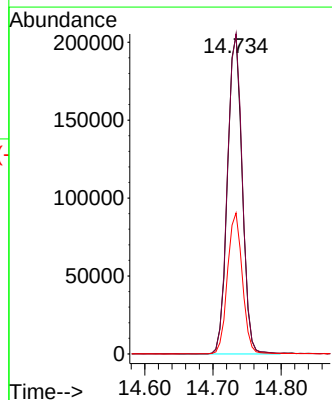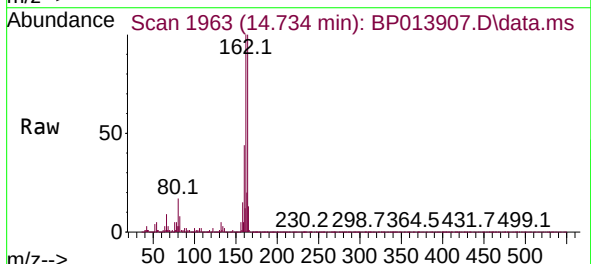

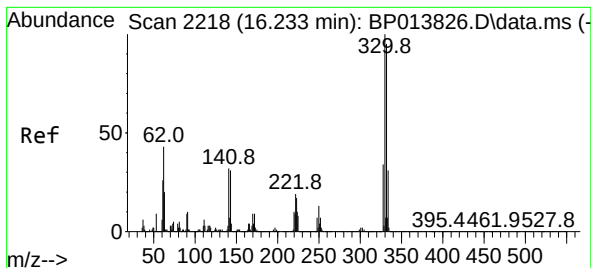

#42

2,4,6-Tribromophenol

Concen: 63.009 ng

RT: 16.222 min Scan# 2218

Delta R.T. -0.012 min

Lab File: BP013907.D

Acq: 01 Mar 2023 01:10

Instrument :

BNA_P

ClientSampleId :

HH-CON-8





Tgt Ion:330 Resp: 279006

Ion Ratio Lower Upper

330 100

332 98.2 76.7 115.1

141 31.2 25.1 37.7

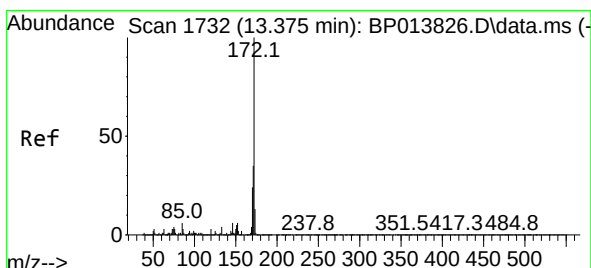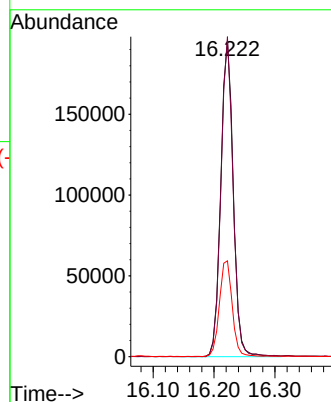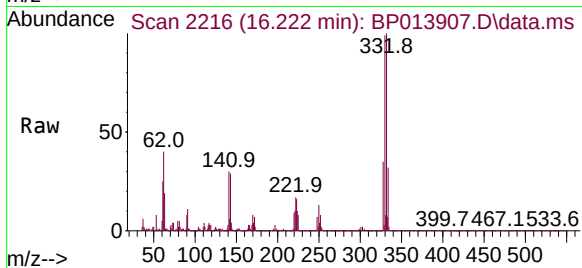

#45

2-Fluorobiphenyl

Concen: 65.562 ng

RT: 13.357 min Scan# 1729

Delta R.T. -0.012 min

Lab File: BP013907.D

Acq: 01 Mar 2023 01:10




Tgt Ion:172 Resp: 1518390


Ion Ratio Lower Upper

172 100

171 35.2 28.2 42.4

170 23.5 19.0 28.4


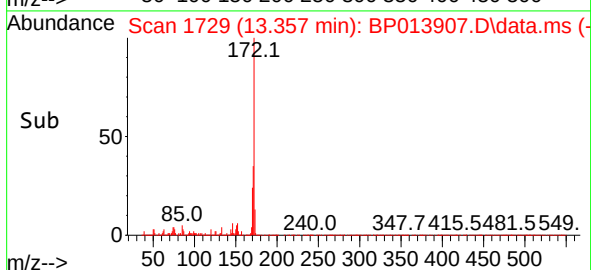
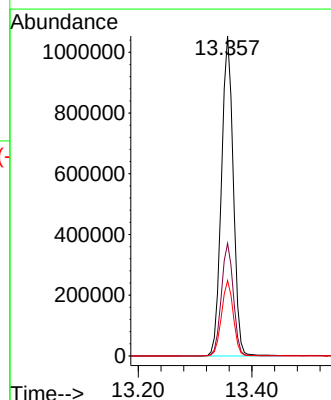
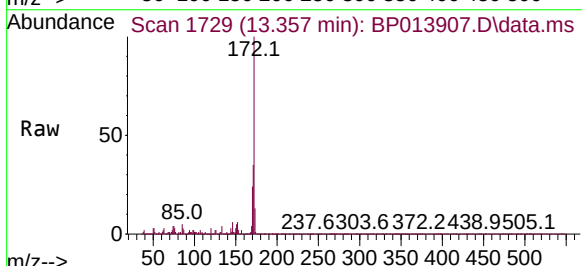




#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.487 min Scan# 2431
Delta R.T. -0.006 min
Lab File: BP013907.D
Acq: 01 Mar 2023 01:10




Instrument :
BNA_P
ClientSampleId :
HH-CON-8


Tgt Ion:188 Resp: 713869
Ion Ratio Lower Upper
188 100
94 7.4 7.0 10.6
80 7.9 7.8 11.8

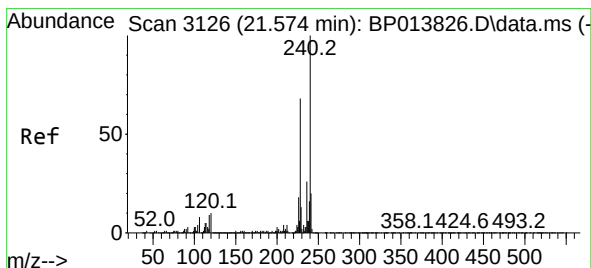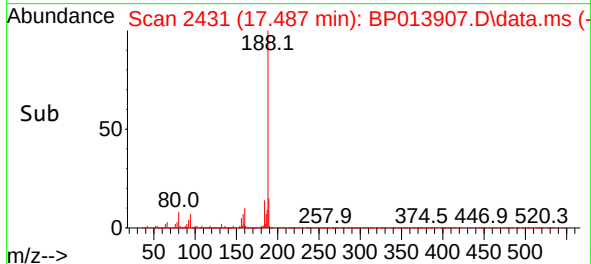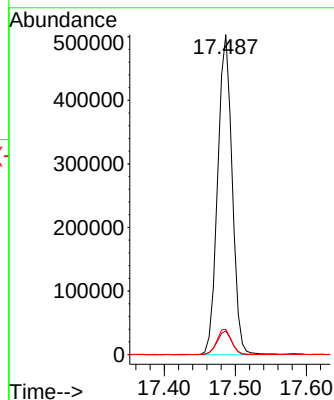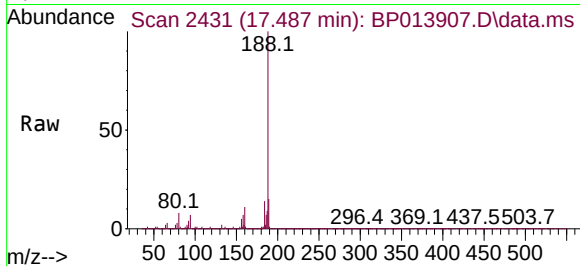

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.563 min Scan# 3124
Delta R.T. -0.012 min
Lab File: BP013907.D
Acq: 01 Mar 2023 01:10

Tgt Ion:240 Resp: 695292
Ion Ratio Lower Upper
240 100
120 8.4 7.9 11.9
236 26.3 20.9 31.3


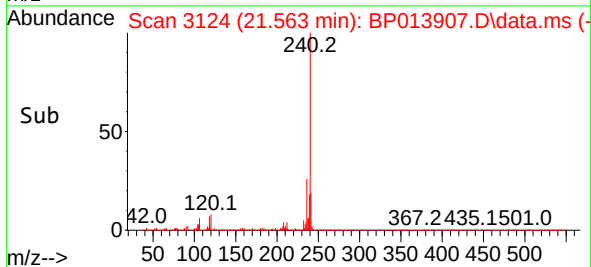
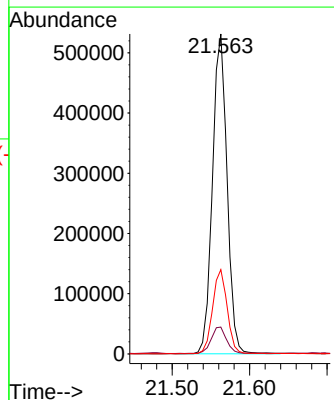
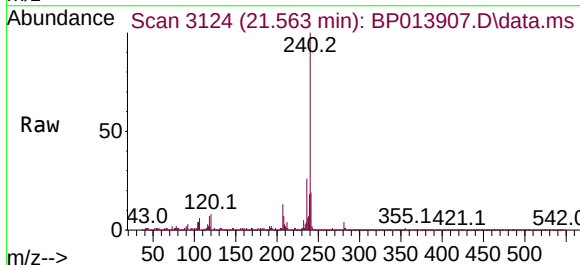


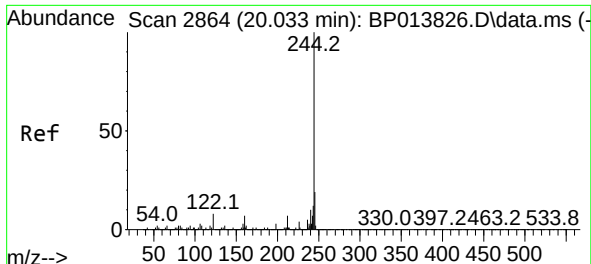

#79
 Terphenyl-d14
 Concen: 76.265 ng
 RT: 20.022 min Scan# 2862
 Delta R.T. -0.006 min
 Lab File: BP013907.D
 Acq: 01 Mar 2023 01:10

Instrument :
 BNA_P
 ClientSampleId :
 HH-CON-8

Tgt Ion:244 Resp: 2756080
 Ion Ratio Lower Upper
 244 100
 212 7.5 5.8 8.6
 122 7.3 6.7 10.1

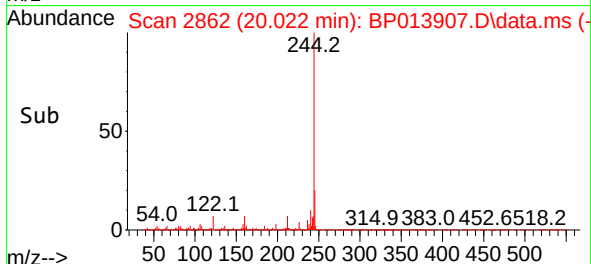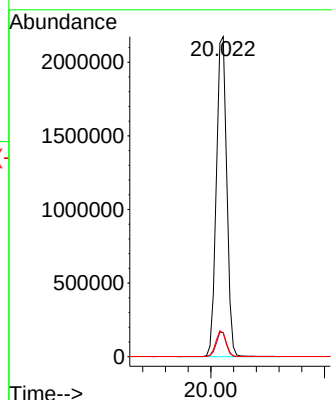

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 24.110 min Scan# 3557
 Delta R.T. -0.012 min
 Lab File: BP013907.D
 Acq: 01 Mar 2023 01:10

Tgt Ion:264 Resp: 803583
 Ion Ratio Lower Upper
 264 100
 260 24.3 19.4 29.0
 265 21.3 17.6 26.4

