
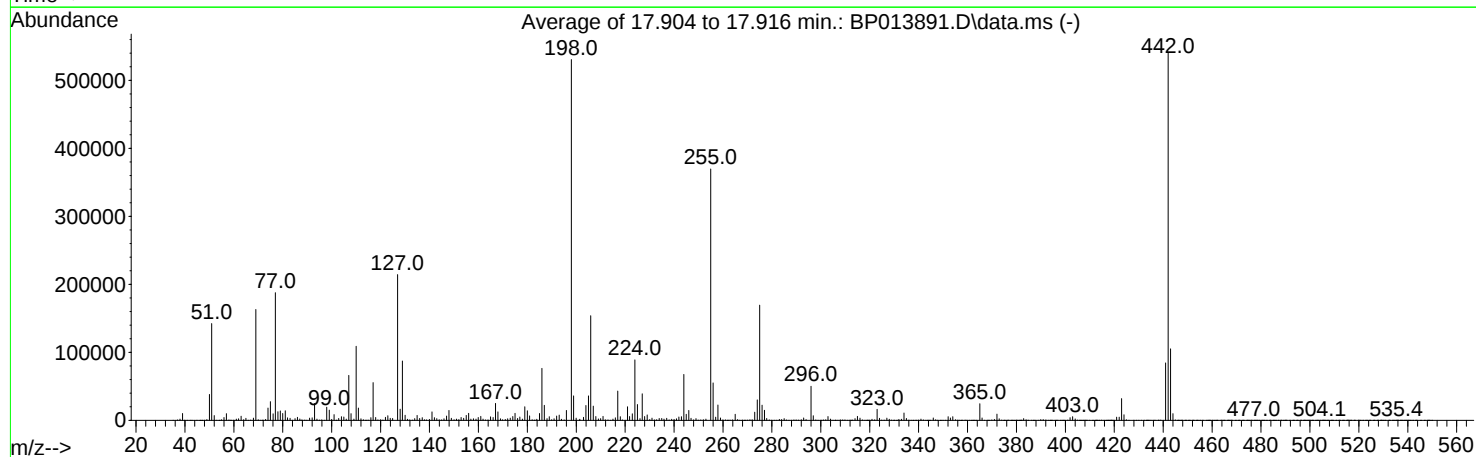


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022823\
 Data File : BP013891.D
 Acq On : 28 Feb 2023 16:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Feb 24 16:57:00 2023

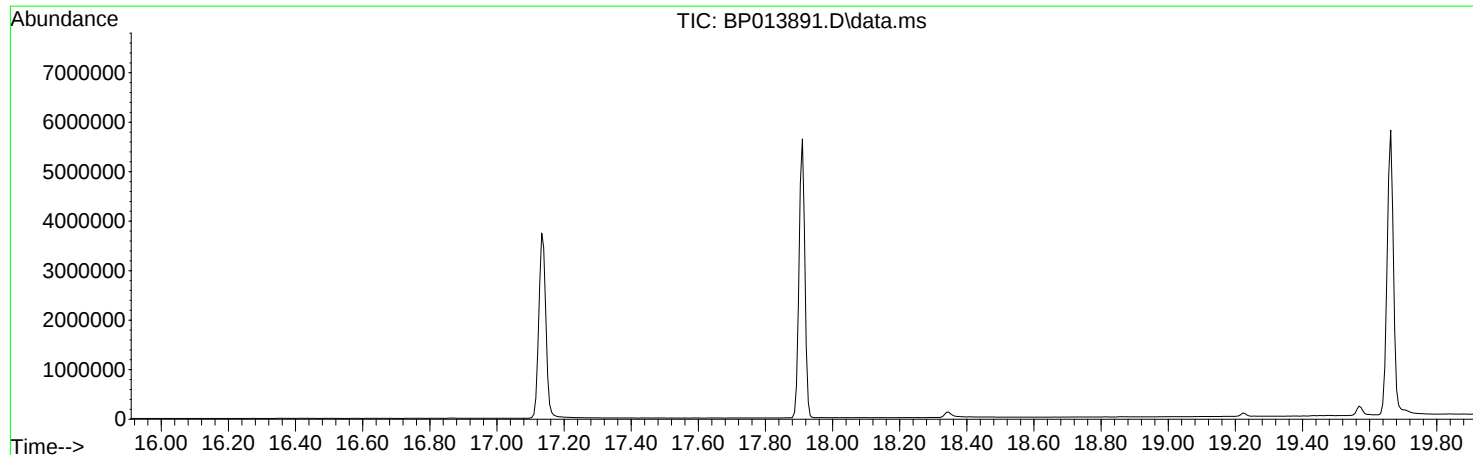




AutoFind: Scans 2502, 2503, 2504; Background Corrected with Scan 2493

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.8	142221	PASS
68	69	0.00	2	1.9	3081	PASS
69	198	0.00	100	30.7	162971	PASS
70	69	0.00	2	0.5	848	PASS
127	198	10	80	40.4	214193	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	530531	PASS
199	198	5	9	6.8	35893	PASS
275	198	10	60	31.9	169222	PASS
365	198	1	100	4.6	24368	PASS
441	198	0.01	100	15.9	84288	PASS
442	442	100	100	100.0	541056	PASS
443	442	15	24	19.4	105142	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022823\
Data File : BP013891.D
Acq On : 28 Feb 2023 16:01
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 01 04:33:22 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 24 16:57:00 2023
Response via : Initial Calibration

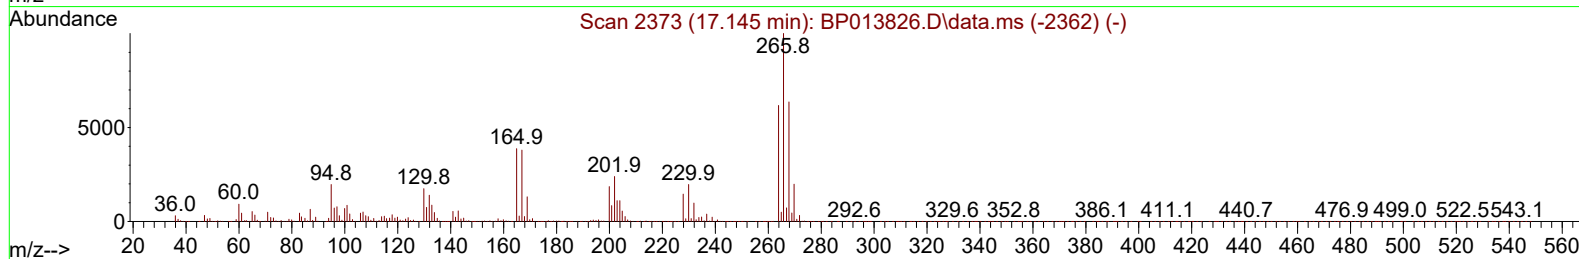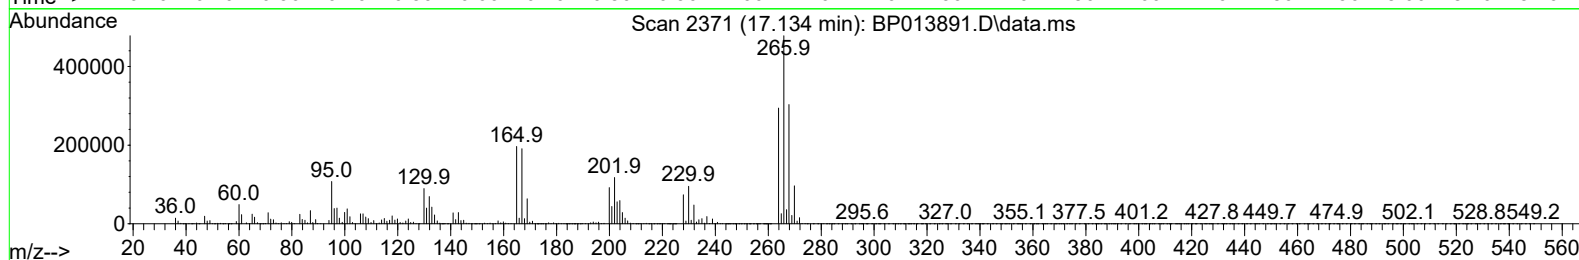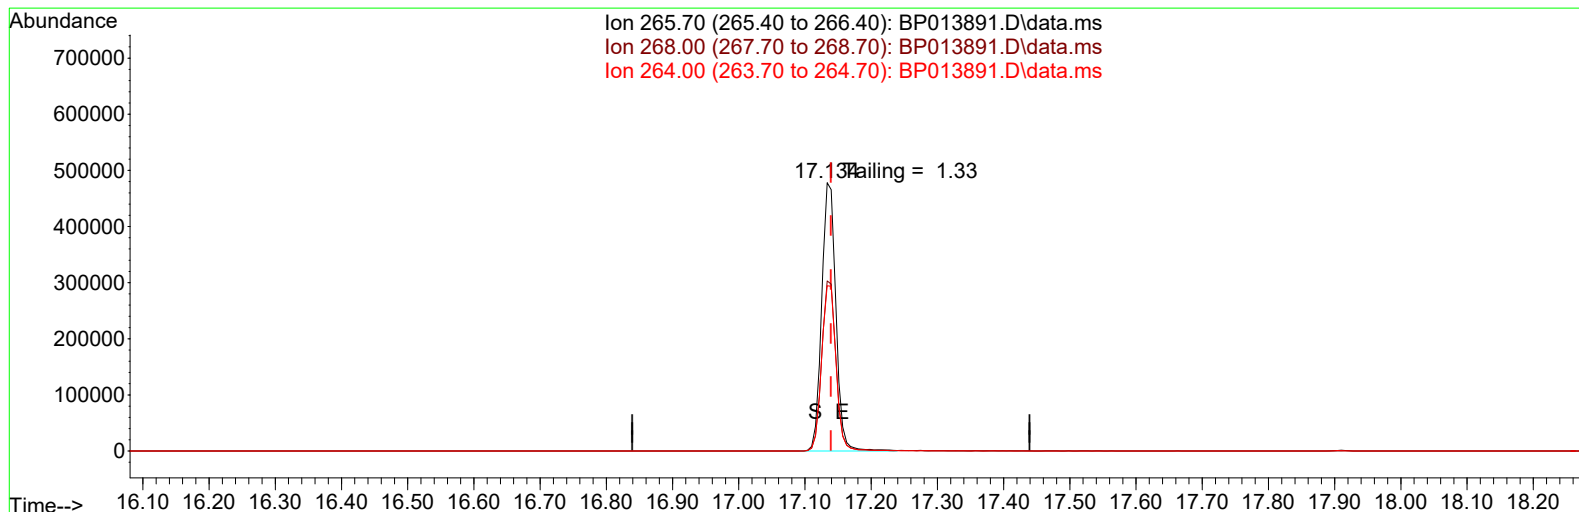

TIC: BP013891.D\data.ms

(70) Pentachlorophenol (C)

17.134min (-0.006) 505435.02 ng




response 710577

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.38
264.00	61.70	61.58
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP022823\
 Data File : BP013891.D
 Acq On : 28 Feb 2023 16:01
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 01 04:33:22 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 24 16:57:00 2023
 Response via : Initial Calibration

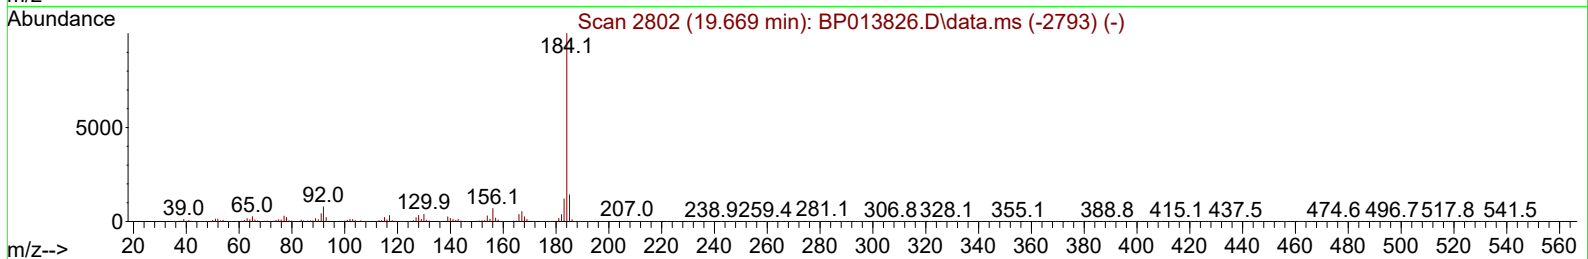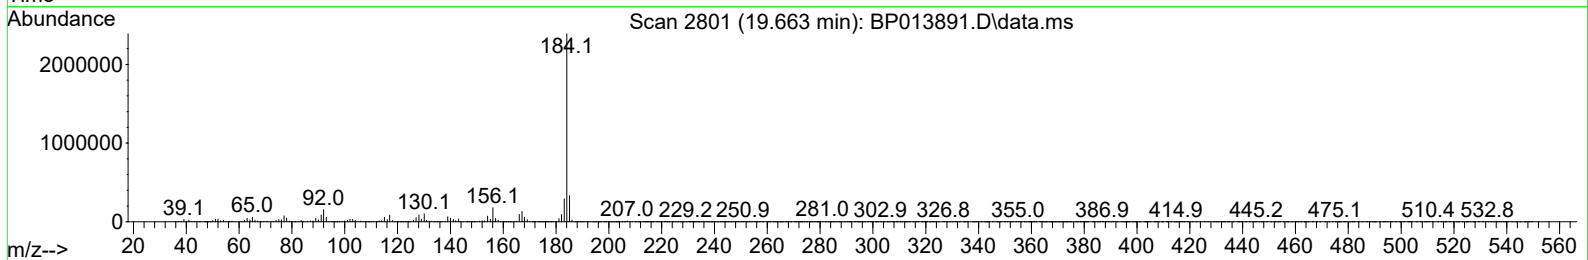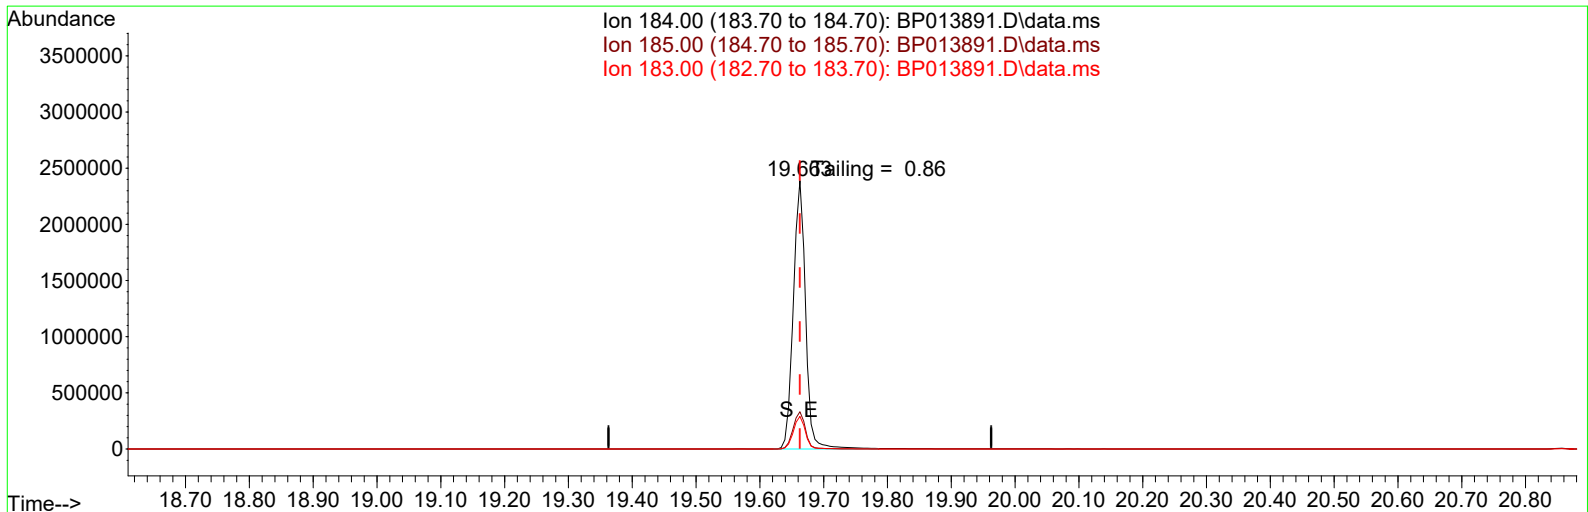

TIC: BP013891.D\data.ms

(77) Benzidine

19.663min (+ 0.000) 138977.71 ng

response 3199622

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.90
183.00	12.00	12.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
2/28/2023	BNA_P	<u>BP013891.D</u>
Compound Name	Response	Retention Time
DDT	1813995	20.857
DDD	22801	20.474
DDE	1084	19.933
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
23885	1837880	1.30

Instrument :
BNA_P
ClientSampleId :
DFTPP