
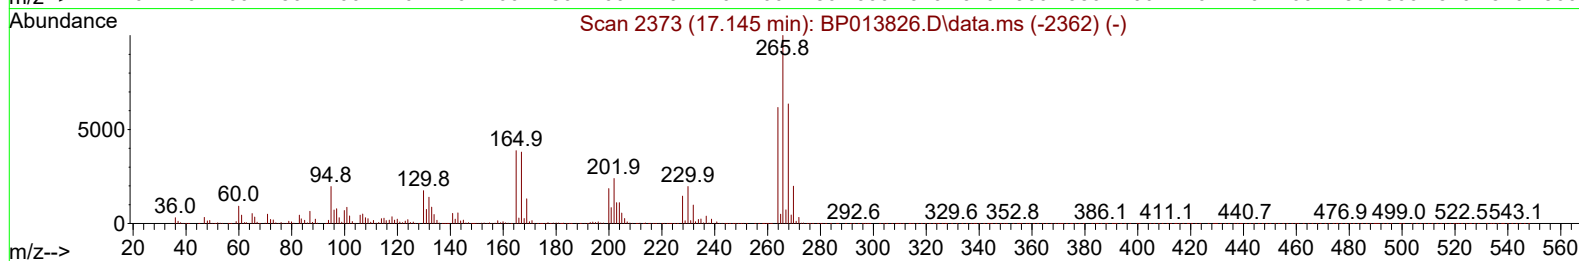
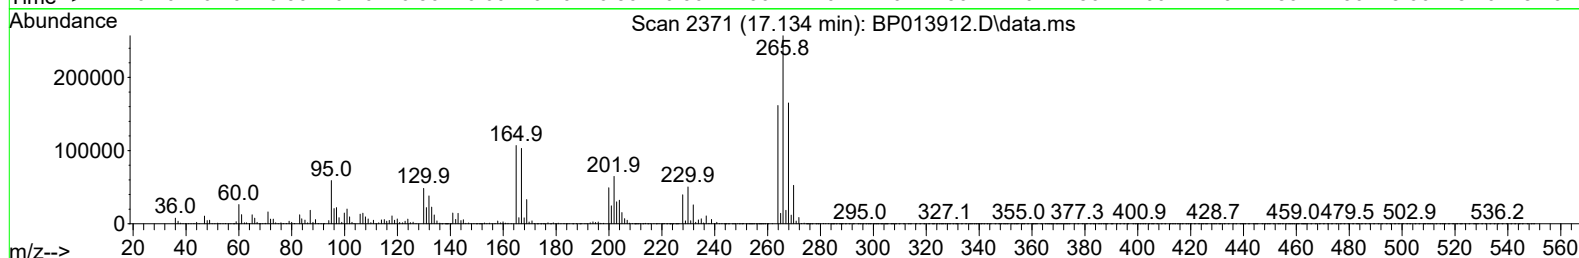


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030123\
Data File : BP013912.D
Acq On : 01 Mar 2023 10:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 02 06:00:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 02 04:26:35 2023
Response via : Initial Calibration

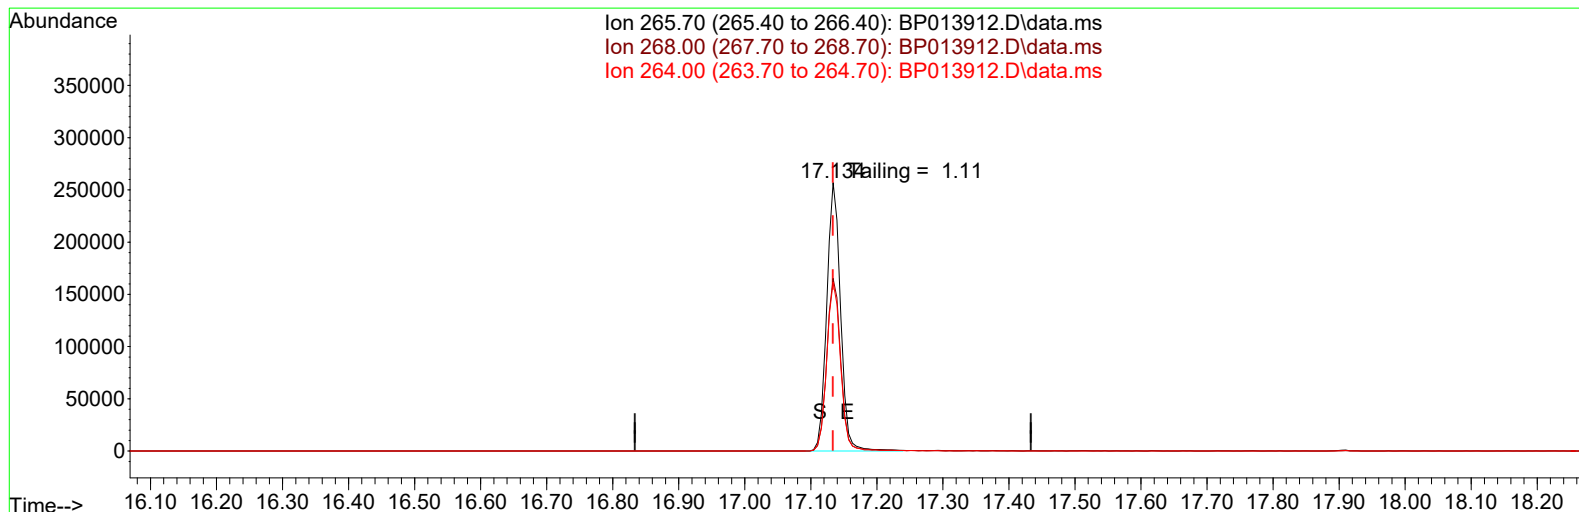

TIC: BP013912.D\data.ms

(70) Pentachlorophenol (C)




17.134min (+ 0.000) 635708.08 ng

response 374398

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.26
264.00	61.70	62.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030123\
Data File : BP013912.D
Acq On : 01 Mar 2023 10:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 02 06:00:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 02 04:26:35 2023
Response via : Initial Calibration

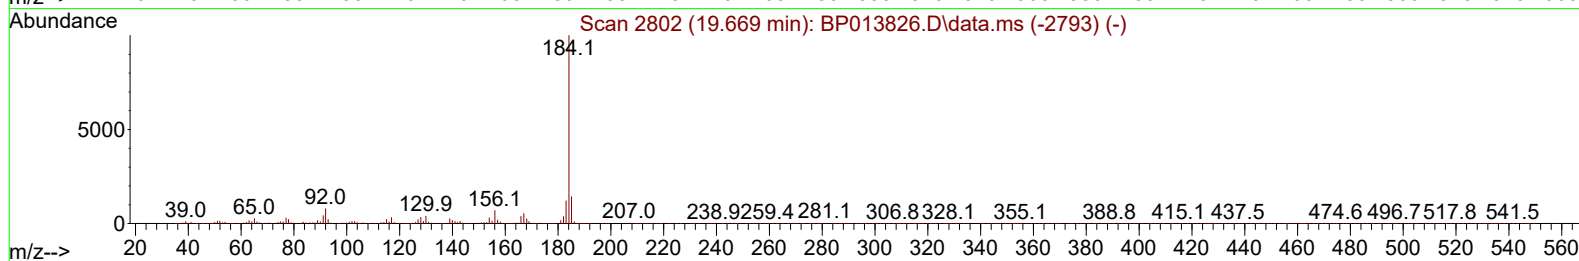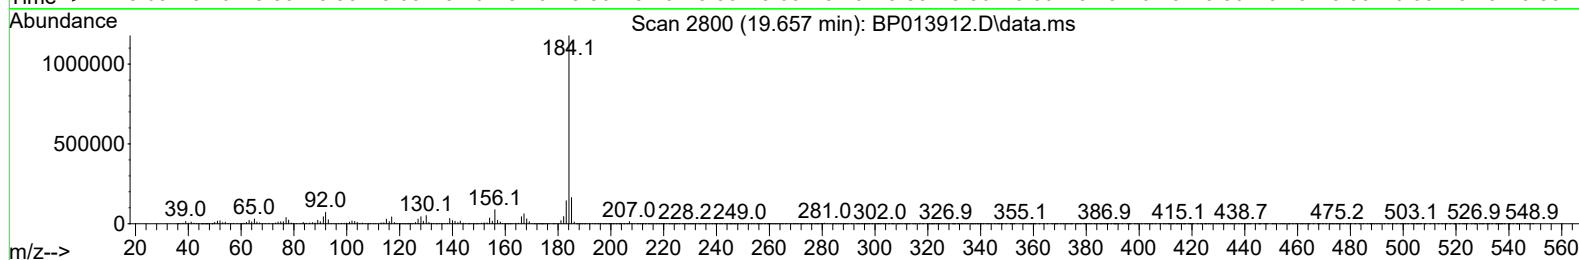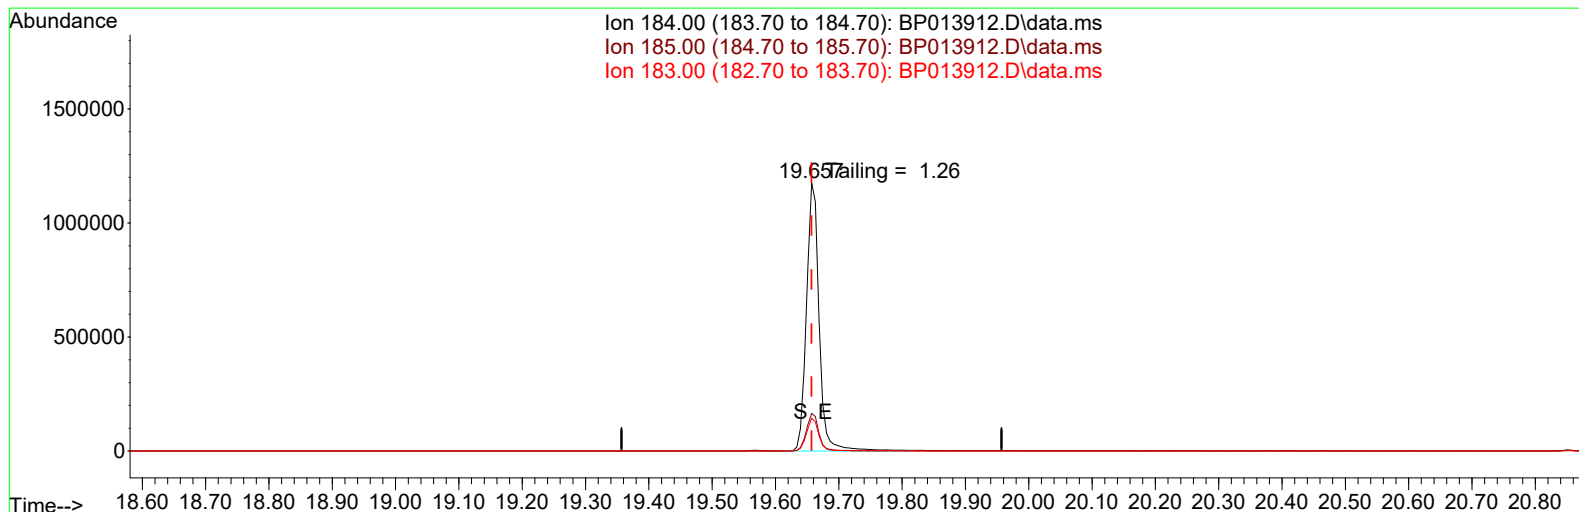

TIC: BP013912.D\data.ms

(77) Benzidine**19.657min (+ 0.000) 488156.90 ng****response 1654914**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.00
183.00	12.00	12.23
0.00	0.00	0.00