


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030123\
 Data File : BP013912.D
 Acq On : 01 Mar 2023 10:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 02 04:26:35 2023

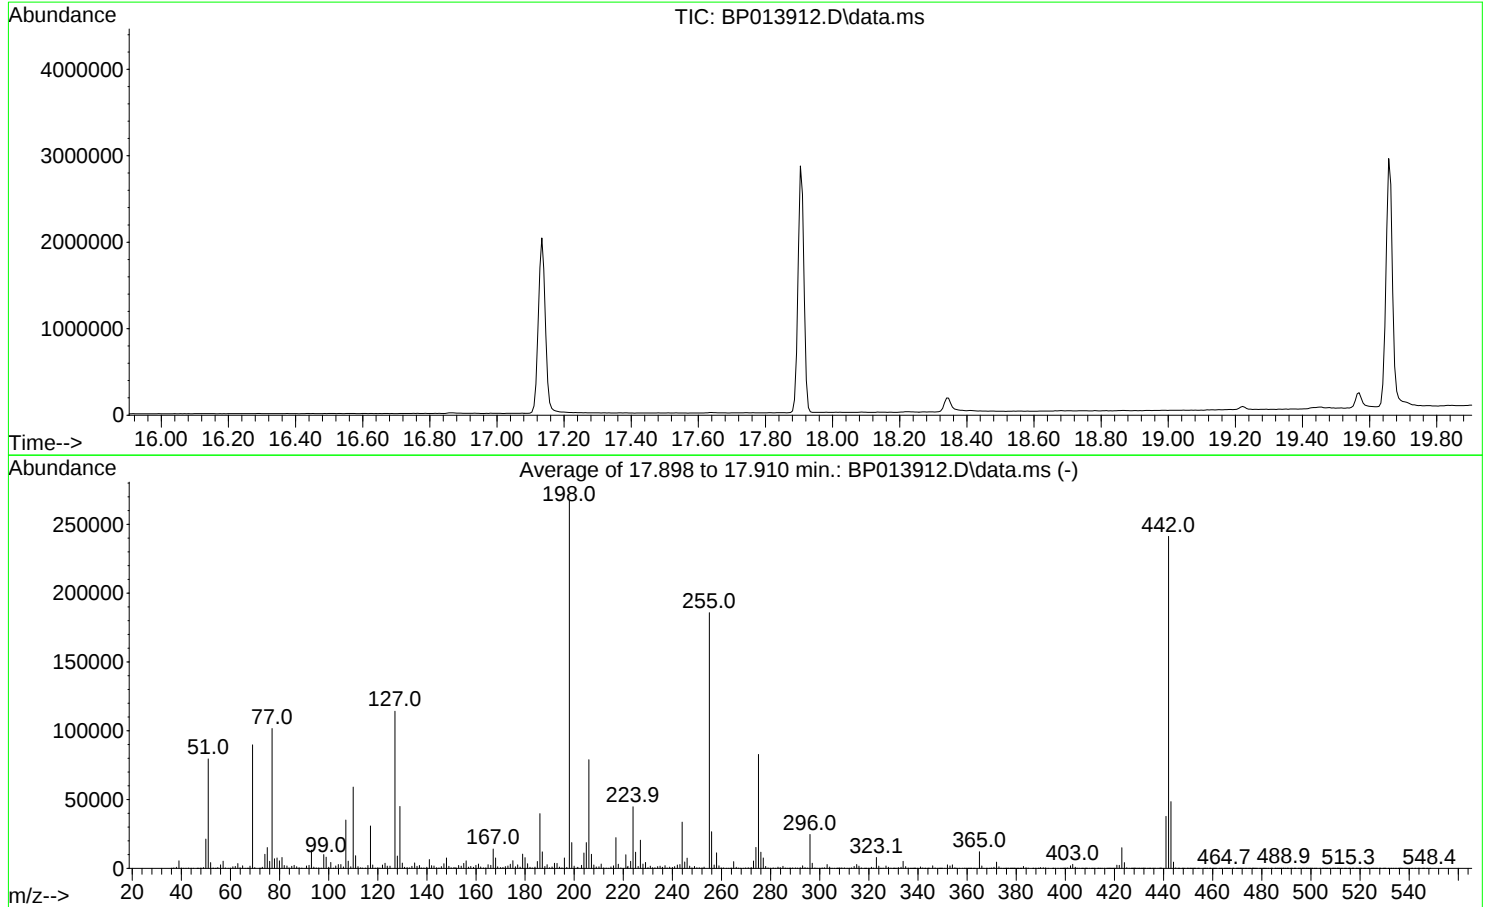




AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.7	79444	PASS
68	69	0.00	2	1.8	1580	PASS
69	198	0.00	100	33.6	89757	PASS
70	69	0.00	2	0.6	577	PASS
127	198	10	80	42.7	114086	PASS
197	198	0.00	2	0.2	665	PASS
198	198	100	100	100.0	267349	PASS
199	198	5	9	7.0	18723	PASS
275	198	10	60	30.9	82688	PASS
365	198	1	100	4.5	12111	PASS
441	198	0.01	100	14.1	37758	PASS
442	442	100	100	100.0	241280	PASS
443	442	15	24	20.1	48488	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030123\
 Data File : BP013912.D
 Acq On : 01 Mar 2023 10:19
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 02 06:00:20 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 02 04:26:35 2023
 Response via : Initial Calibration

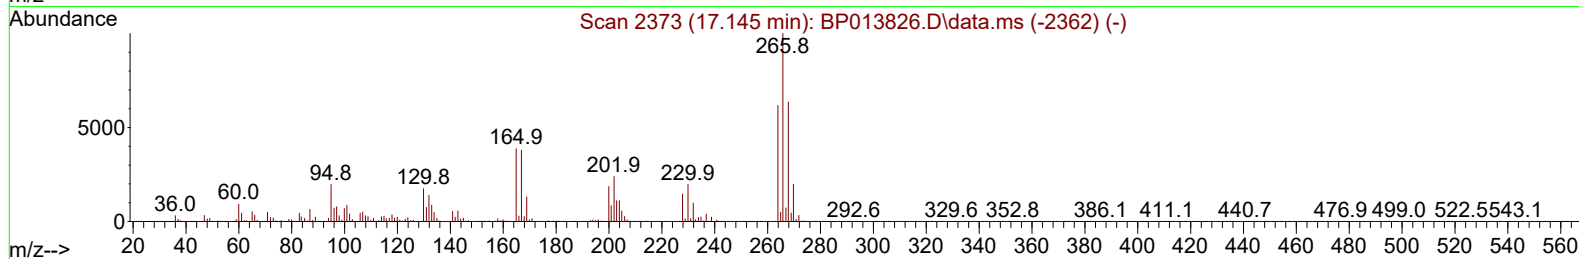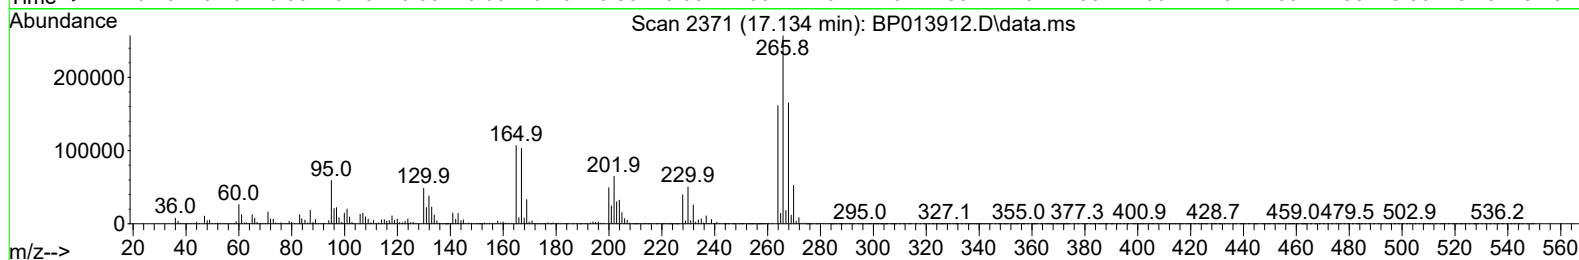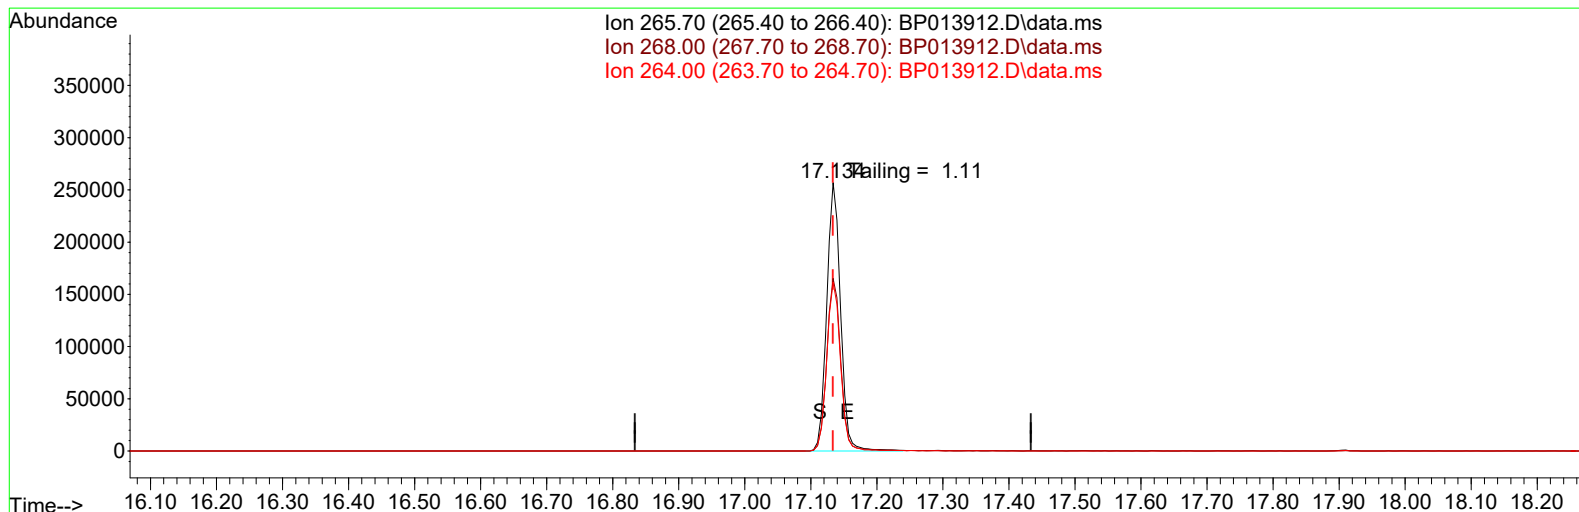

TIC: BP013912.D\data.ms

(70) Pentachlorophenol (C)

17.134min (+ 0.000) 635708.08 ng




response 374398

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	64.26
264.00	61.70	62.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030123\
Data File : BP013912.D
Acq On : 01 Mar 2023 10:19
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 02 06:00:20 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 02 04:26:35 2023
Response via : Initial Calibration

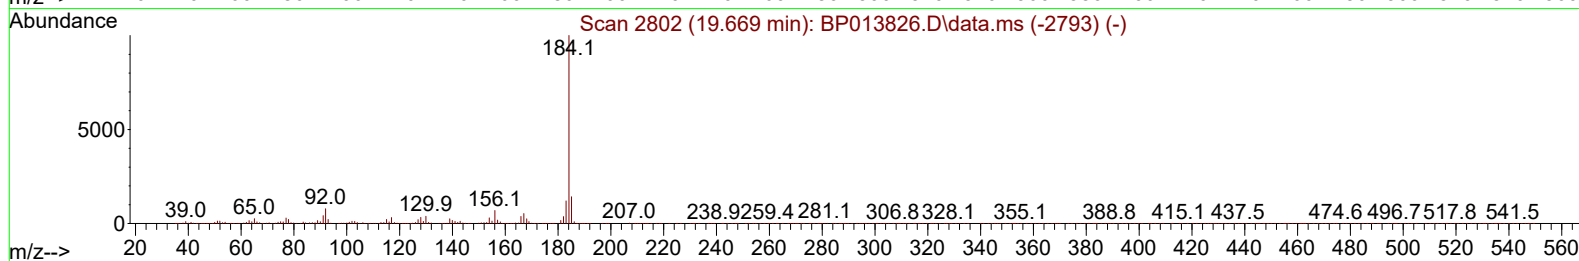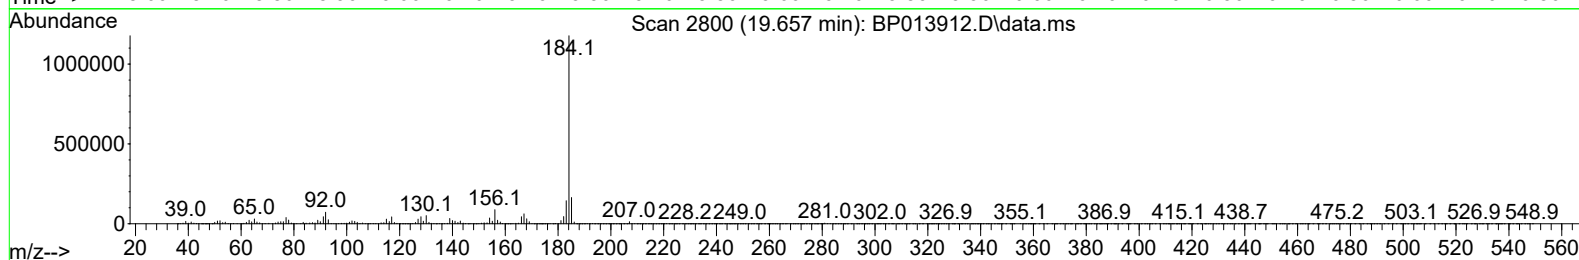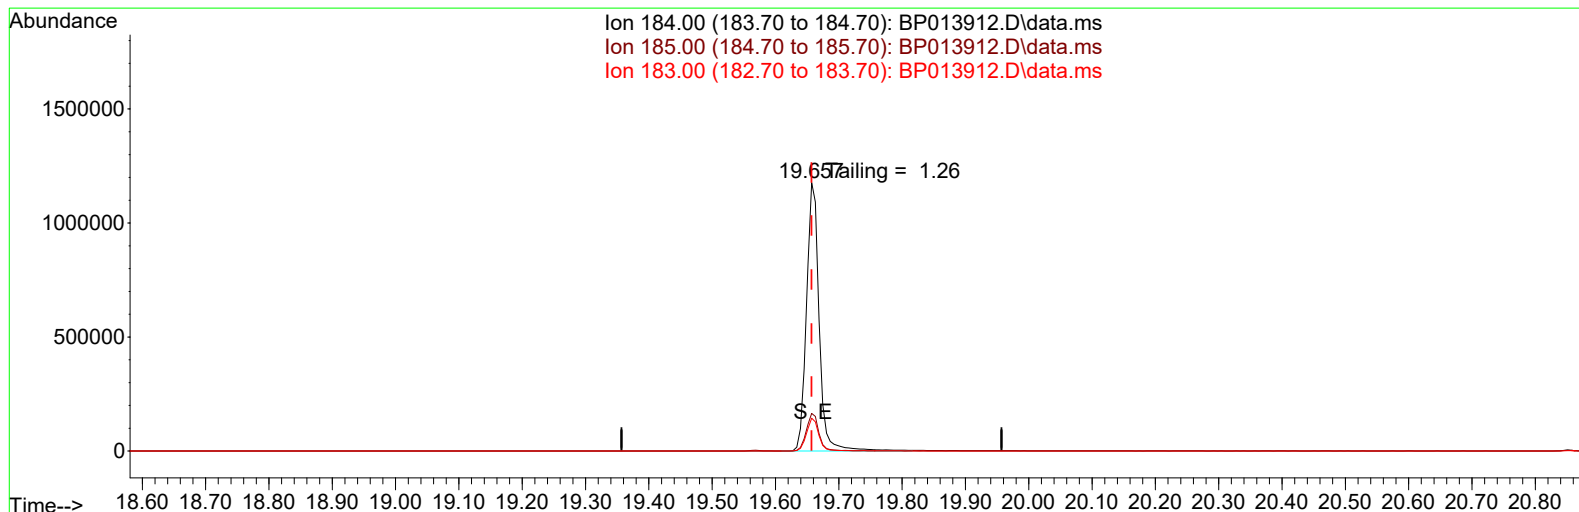

TIC: BP013912.D\data.ms

(77) Benzidine

19.657min (+ 0.000) 488156.90 ng

response 1654914

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.00
183.00	12.00	12.23
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/1/2023	BNA_P	<u>BP013912.D</u>
Compound Name	Response	Retention Time
DDT	976616	20.851
DDD	13656	20.475
DDE	718	19.928
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14374	990990	1.45

Instrument :
BNA_P
ClientSampleId :
DFTPP