
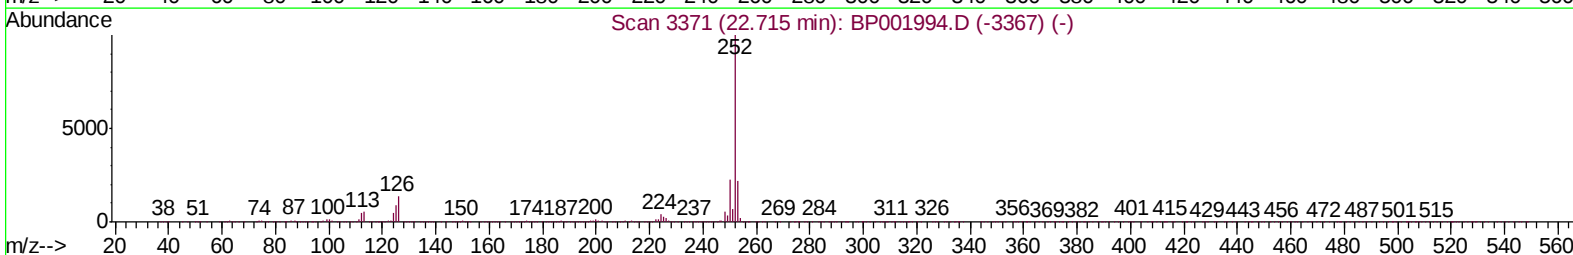
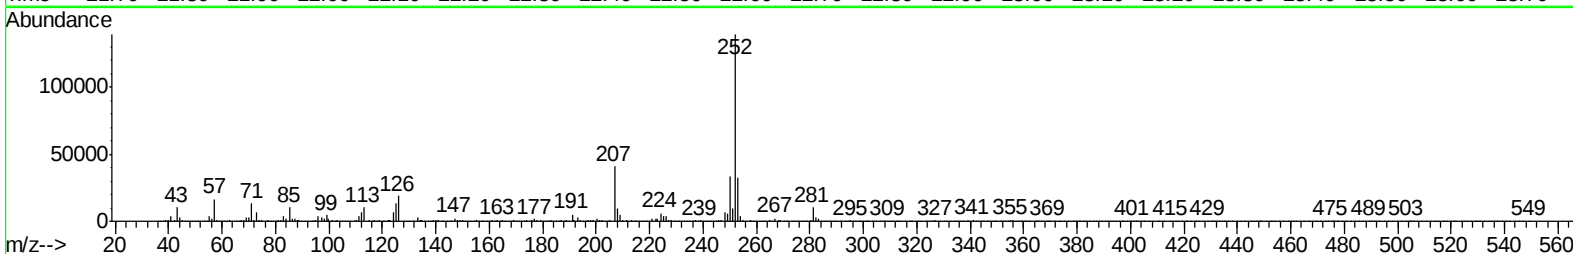


Data File : BP001996.D
Acq On : 02 Mar 2020 18:43
Operator : CG/JU
Sample : L1543-19DL 5X
Misc :
ALS Vial : 14 Sample Multiplier: 1

Quant Time: Mar 03 03:54:20 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 03:51:53 2020
Response via : Initial Calibration

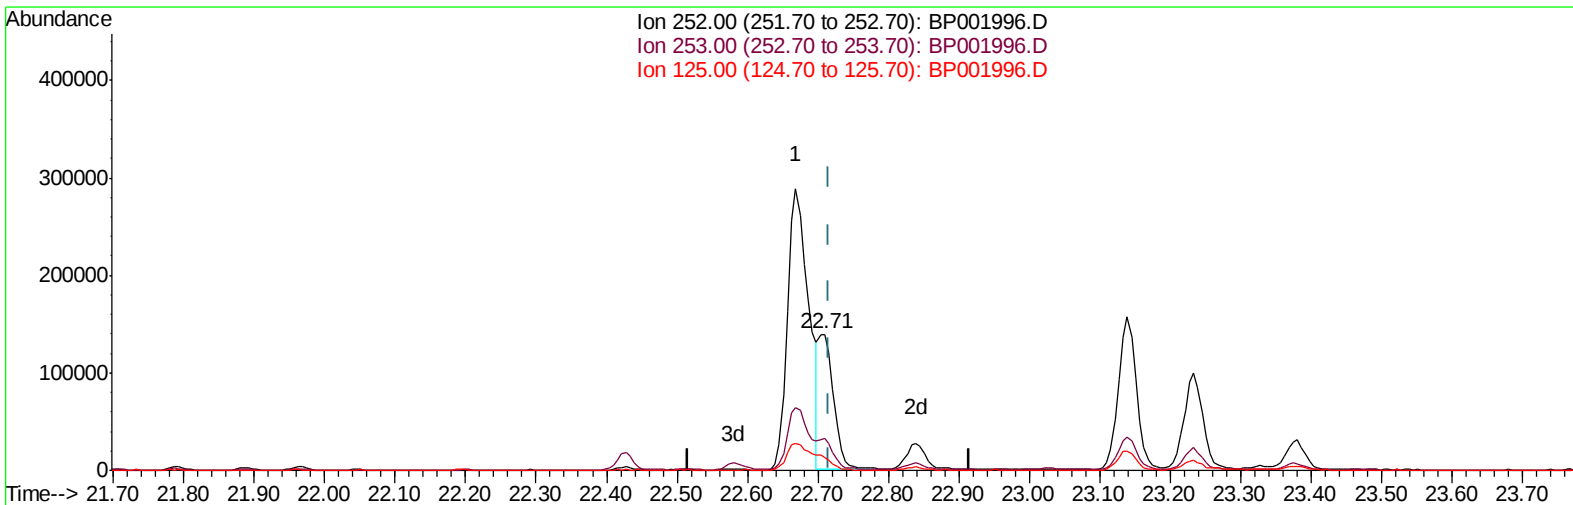

TIC: BP001996.D

(89) Benzo(k)fluoranthene

22.710min (-0.006) 1.78ng/ul m

response 197518

Ion	Exp%	Act%
252.00	100	100
253.00	21.90	23.41
125.00	9.20	9.85
0.00	0.00	0.00