
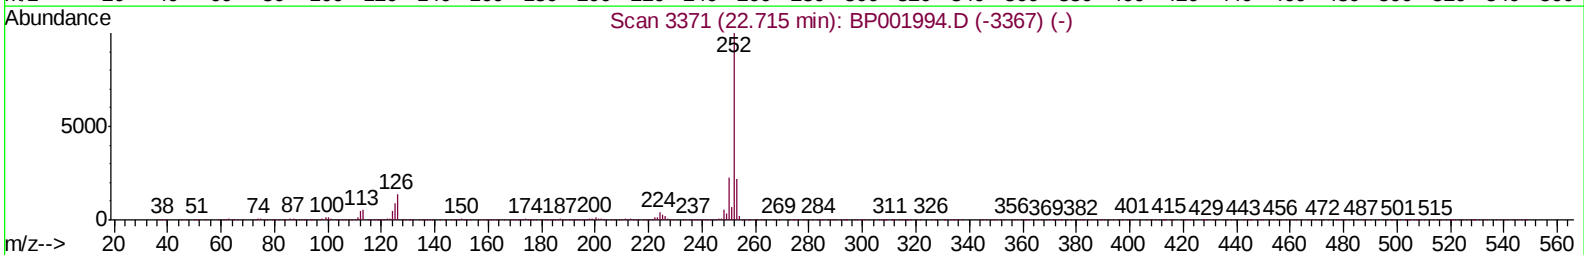
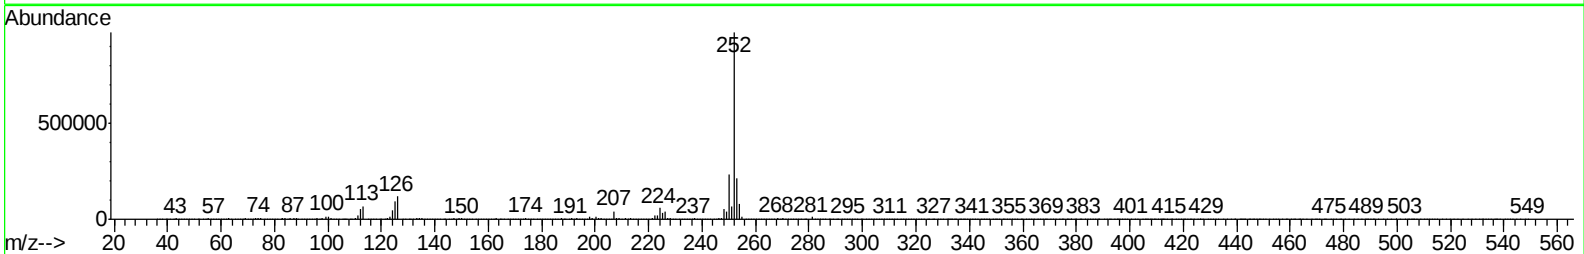


Data File : BP002002.D
Acq On : 02 Mar 2020 22:06
Operator : CG/JU
Sample : L1616-10
Misc :
ALS Vial : 20 Sample Multiplier: 1

Quant Time: Mar 03 03:55:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 03:51:53 2020
Response via : Initial Calibration

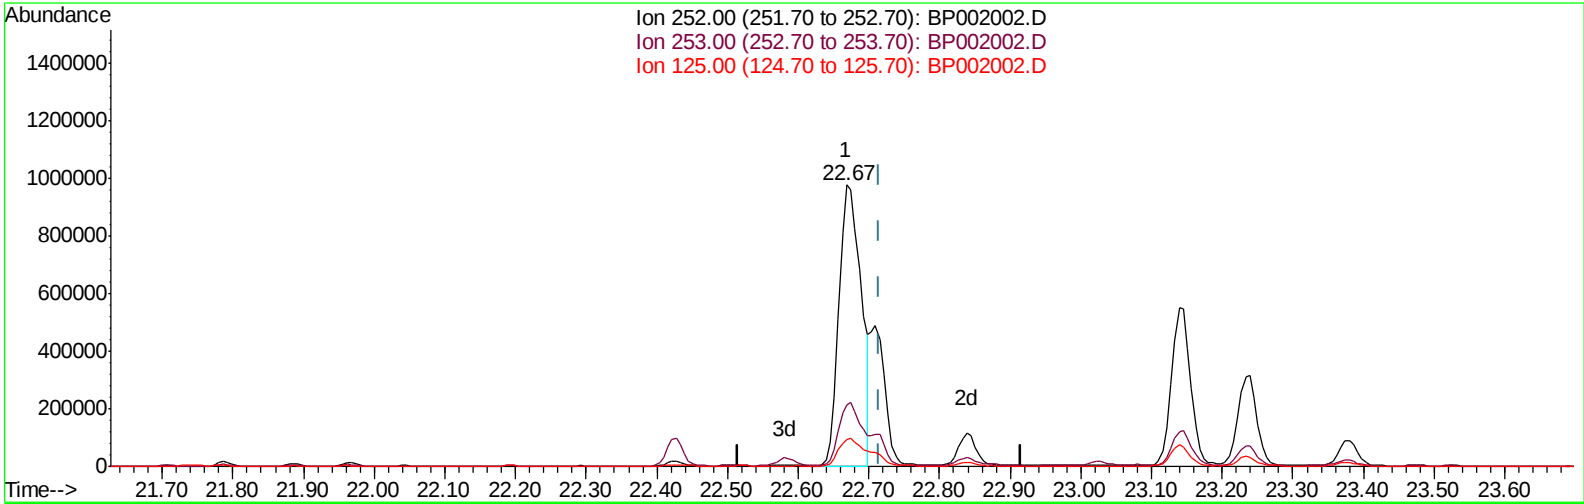

TIC: BP002002.D

(89) Benzo(k)fluoranthene
22.668min (-0.047) 20.16ng/ul
response 2143882

Ion	Exp%	Act%
252.00	100	100
253.00	21.90	22.01
125.00	9.20	9.78
0.00	0.00	0.00