
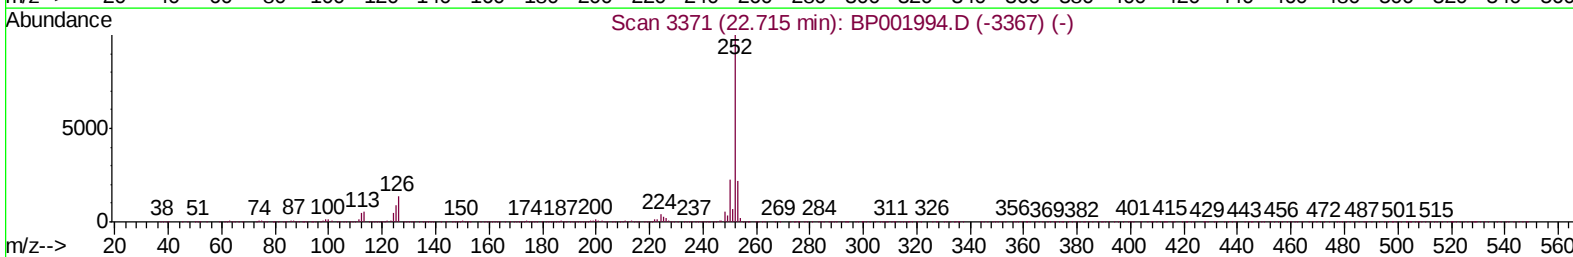
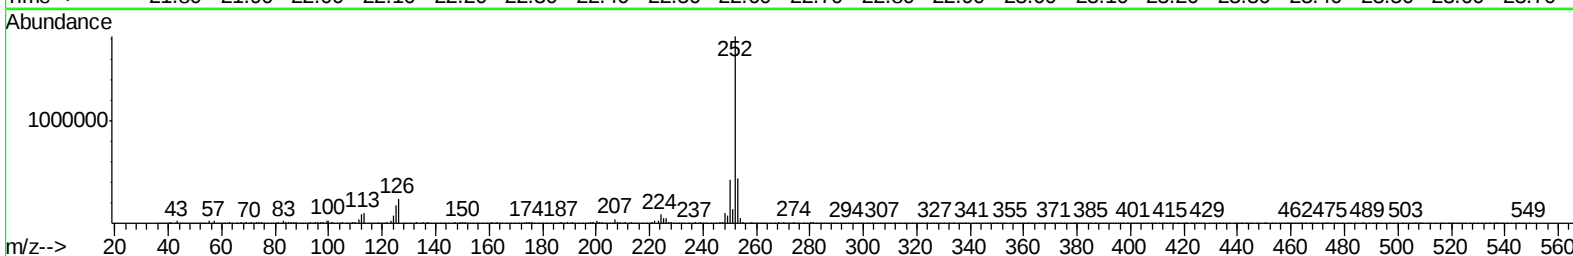


Data File : BP002006.D
Acq On : 03 Mar 2020 00:22
Operator : CG/JU
Sample : L1616-14
Misc :
ALS Vial : 24 Sample Multiplier: 1

Quant Time: Mar 03 03:56:27 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 03:51:53 2020
Response via : Initial Calibration

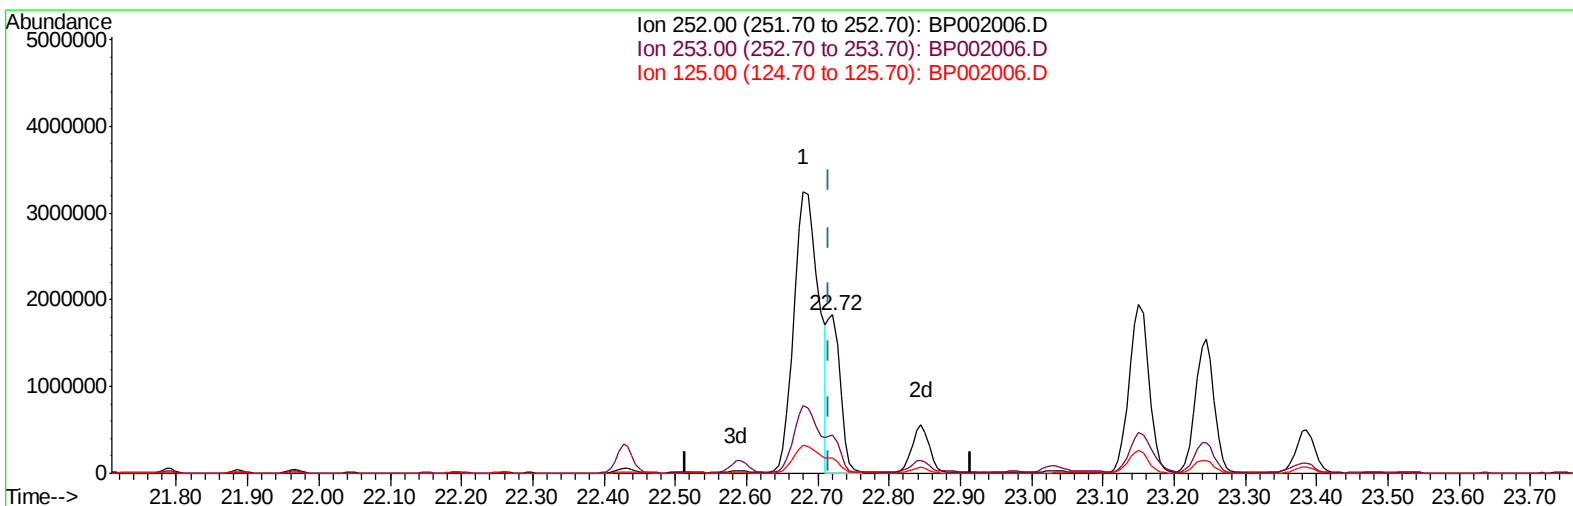

TIC: BP002006.D

(89) Benzo(k)fluoranthene

22.721min (+0.006) 26.20ng/ul m

response 2321823

Ion	Exp%	Act%
252.00	100	100
253.00	21.90	23.99
125.00	9.20	9.40
0.00	0.00	0.00