
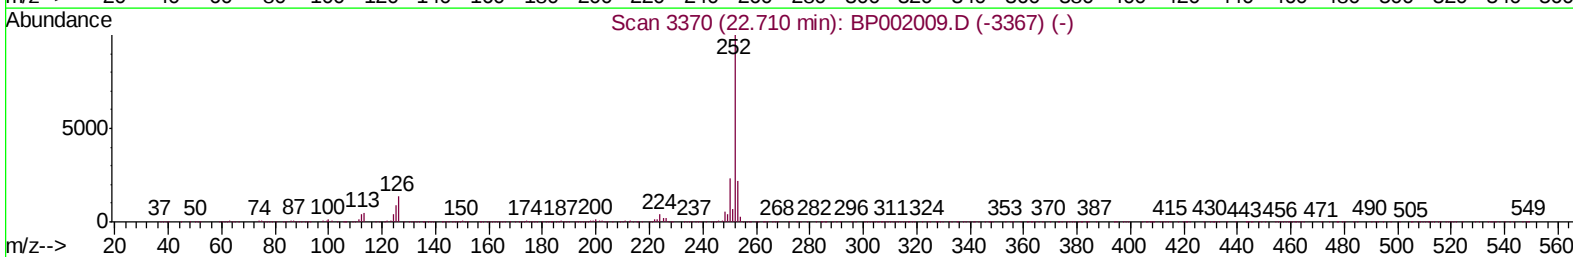
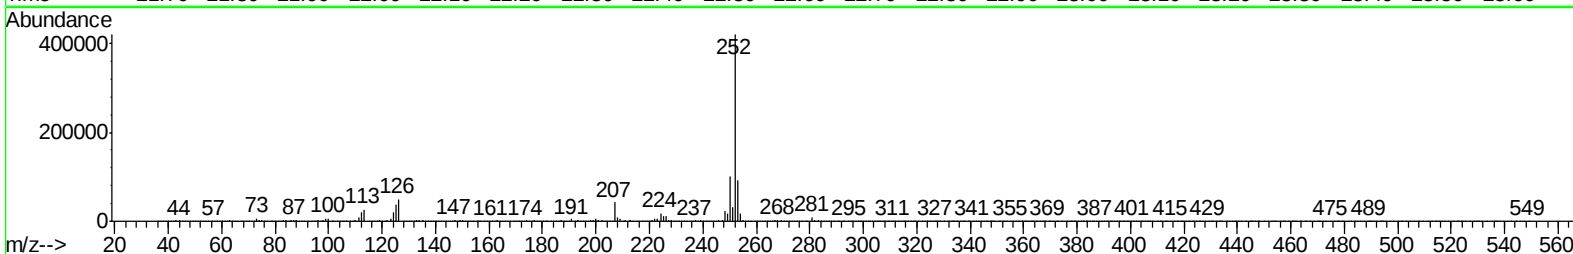


Data File : BP002012.D
Acq On : 03 Mar 2020 04:19
Operator : CG/JU
Sample : L1616-19
Misc :
ALS Vial : 29 Sample Multiplier: 1

Quant Time: Mar 03 05:33:33 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 05:31:15 2020
Response via : Initial Calibration

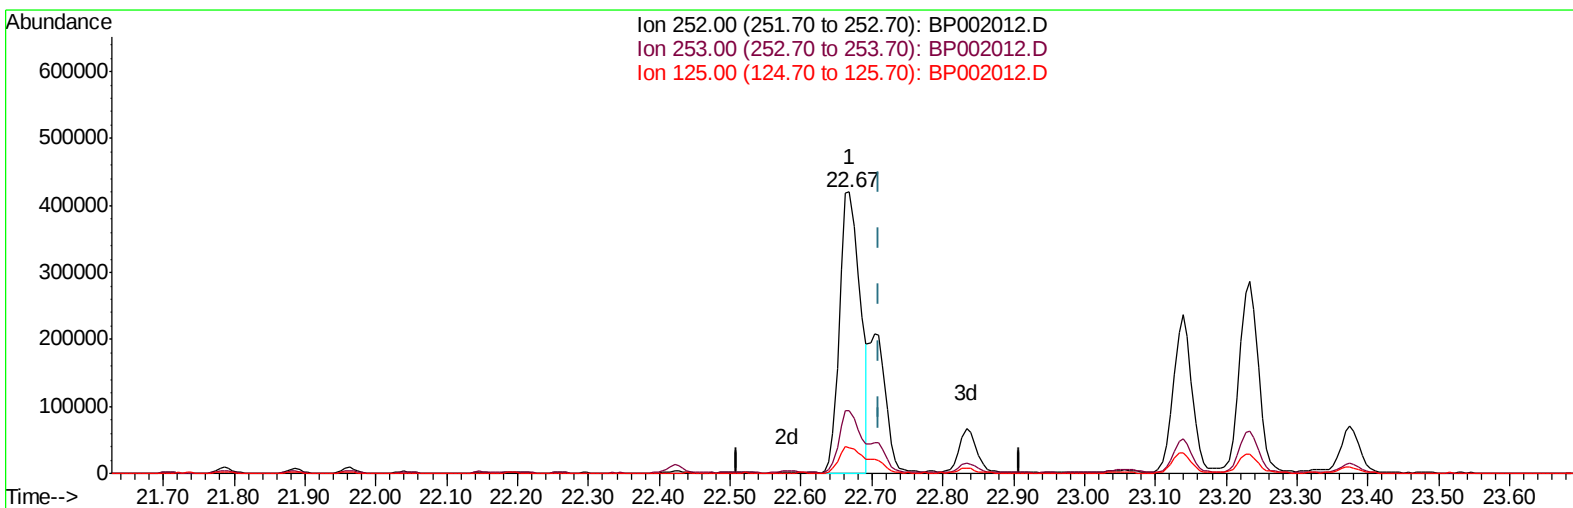

TIC: BP002012.D

(89) Benzo(k)fluoranthene
22.669min (-0.041) 7.29ng/ul
response 868407

Ion	Exp%	Act%
252.00	100	100
253.00	21.90	22.25
125.00	9.20	9.16
0.00	0.00	0.00