

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030220\
 Data File : BP001995.D
 Acq On : 02 Mar 2020 18:09
 Operator : CG/JU
 Sample : L1616-06
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBDQ0

Quant Time: Mar 03 03:54:10 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 03:51:53 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	258946	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1054599	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	664183	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1432155	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1402999	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1613813	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.17	96	32644	5.42	ng/uL	0.00
5) Phenol-d5	6.82	99	544616	27.57	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	317195	30.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	485403	28.41	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	447210	27.55	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	219740	27.12	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	241913	26.54	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	462969	26.37	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	618223	32.12	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1429177	28.43	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1732154	28.81	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	176340	18.35	ng/ul	0.00
58) Fluorene-d10	15.27	176	1282754	29.49	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	147364	18.66	ng/ul	0.00
71) Anthracene-d10	17.13	188	1926864	29.94	ng/ul	0.00
79) Pyrene-d10	19.37	212	2221910	30.25	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	2441592	29.57	ng/ul	0.00


Target Compounds				Ovalue	
45) Dimethylphthalate	13.73	163	118029	2.275	ng/ul 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030220\
Data File : BP001995.D
Acq On : 02 Mar 2020 18:09
Operator : CG/JU
Sample : L1616-06
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBDQ0

Quant Time: Mar 03 03:54:10 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 03:51:53 2020
Response via : Initial Calibration

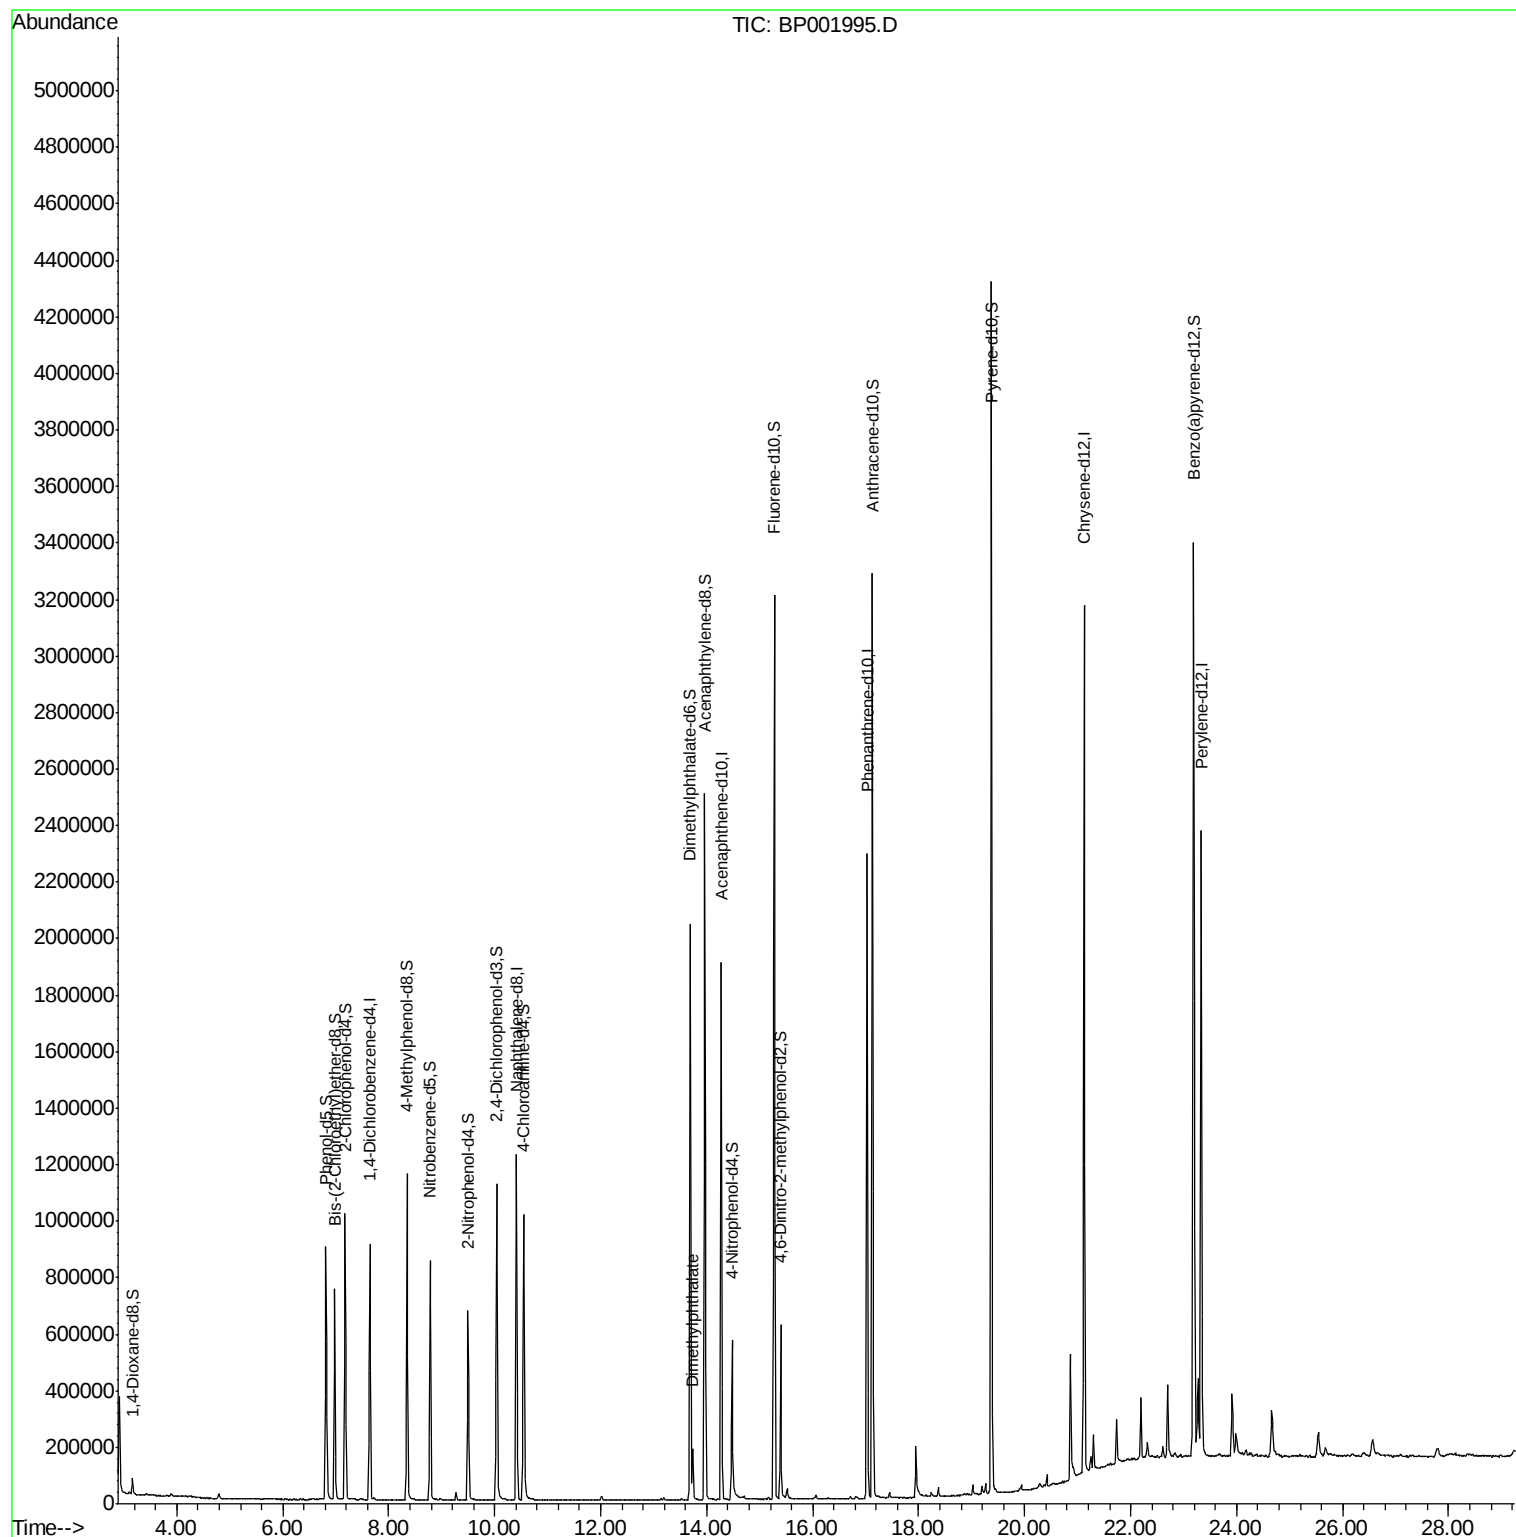

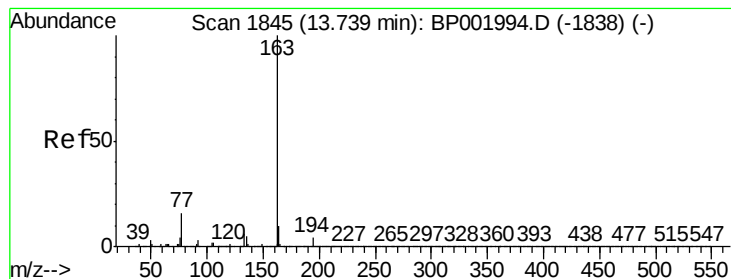

#45

Dimethylphthalate

Concen: 2.275 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BP001995.D

Acq: 02 Mar 2020 18:09

Instrument :

BNA_P

ClientSampleId :

DBDQ0


Tot Ion:163 Resp: 118029

Ion Ratio Lower Upper

163 100

194 4.1 3.6 5.4

164 9.4 8.2 12.4

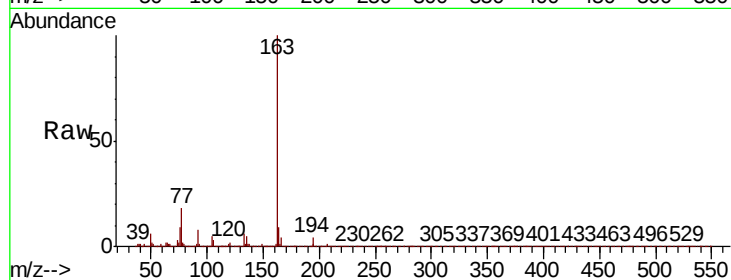

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

