

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030220\
 Data File : BP001999.D
 Acq On : 02 Mar 2020 20:24
 Operator : CG/JU
 Sample : L1616-07
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBDQ1

Quant Time: Mar 03 03:55:02 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 03:51:53 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	284610	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1168435	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	736891	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1616199	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1607289	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1827928	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.17	96	31907	4.82	ng/uL	0.00
5) Phenol-d5	6.82	99	552535	25.45	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	323630	28.15	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	490701	26.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	460371	25.80	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	224623	25.03	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	244145	24.18	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	486224	25.00	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	644307	30.22	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1510482	27.09	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1828077	27.41	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	184964	17.35	ng/ul	0.00
58) Fluorene-d10	15.27	176	1365185	28.29	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	151986	17.06	ng/ul	0.00
71) Anthracene-d10	17.13	188	2055995	28.30	ng/ul	0.00
79) Pyrene-d10	19.37	212	2361437	28.07	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	2572324	27.51	ng/ul	0.00
Target Compounds						
6) Phenol	6.85	94	29261	1.298	ng/ul	94
45) Dimethylphthalate	13.73	163	135028	2.346	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030220\
Data File : BP001999.D
Acq On : 02 Mar 2020 20:24
Operator : CG/JU
Sample : L1616-07
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBDQ1

Quant Time: Mar 03 03:55:02 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 03:51:53 2020
Response via : Initial Calibration

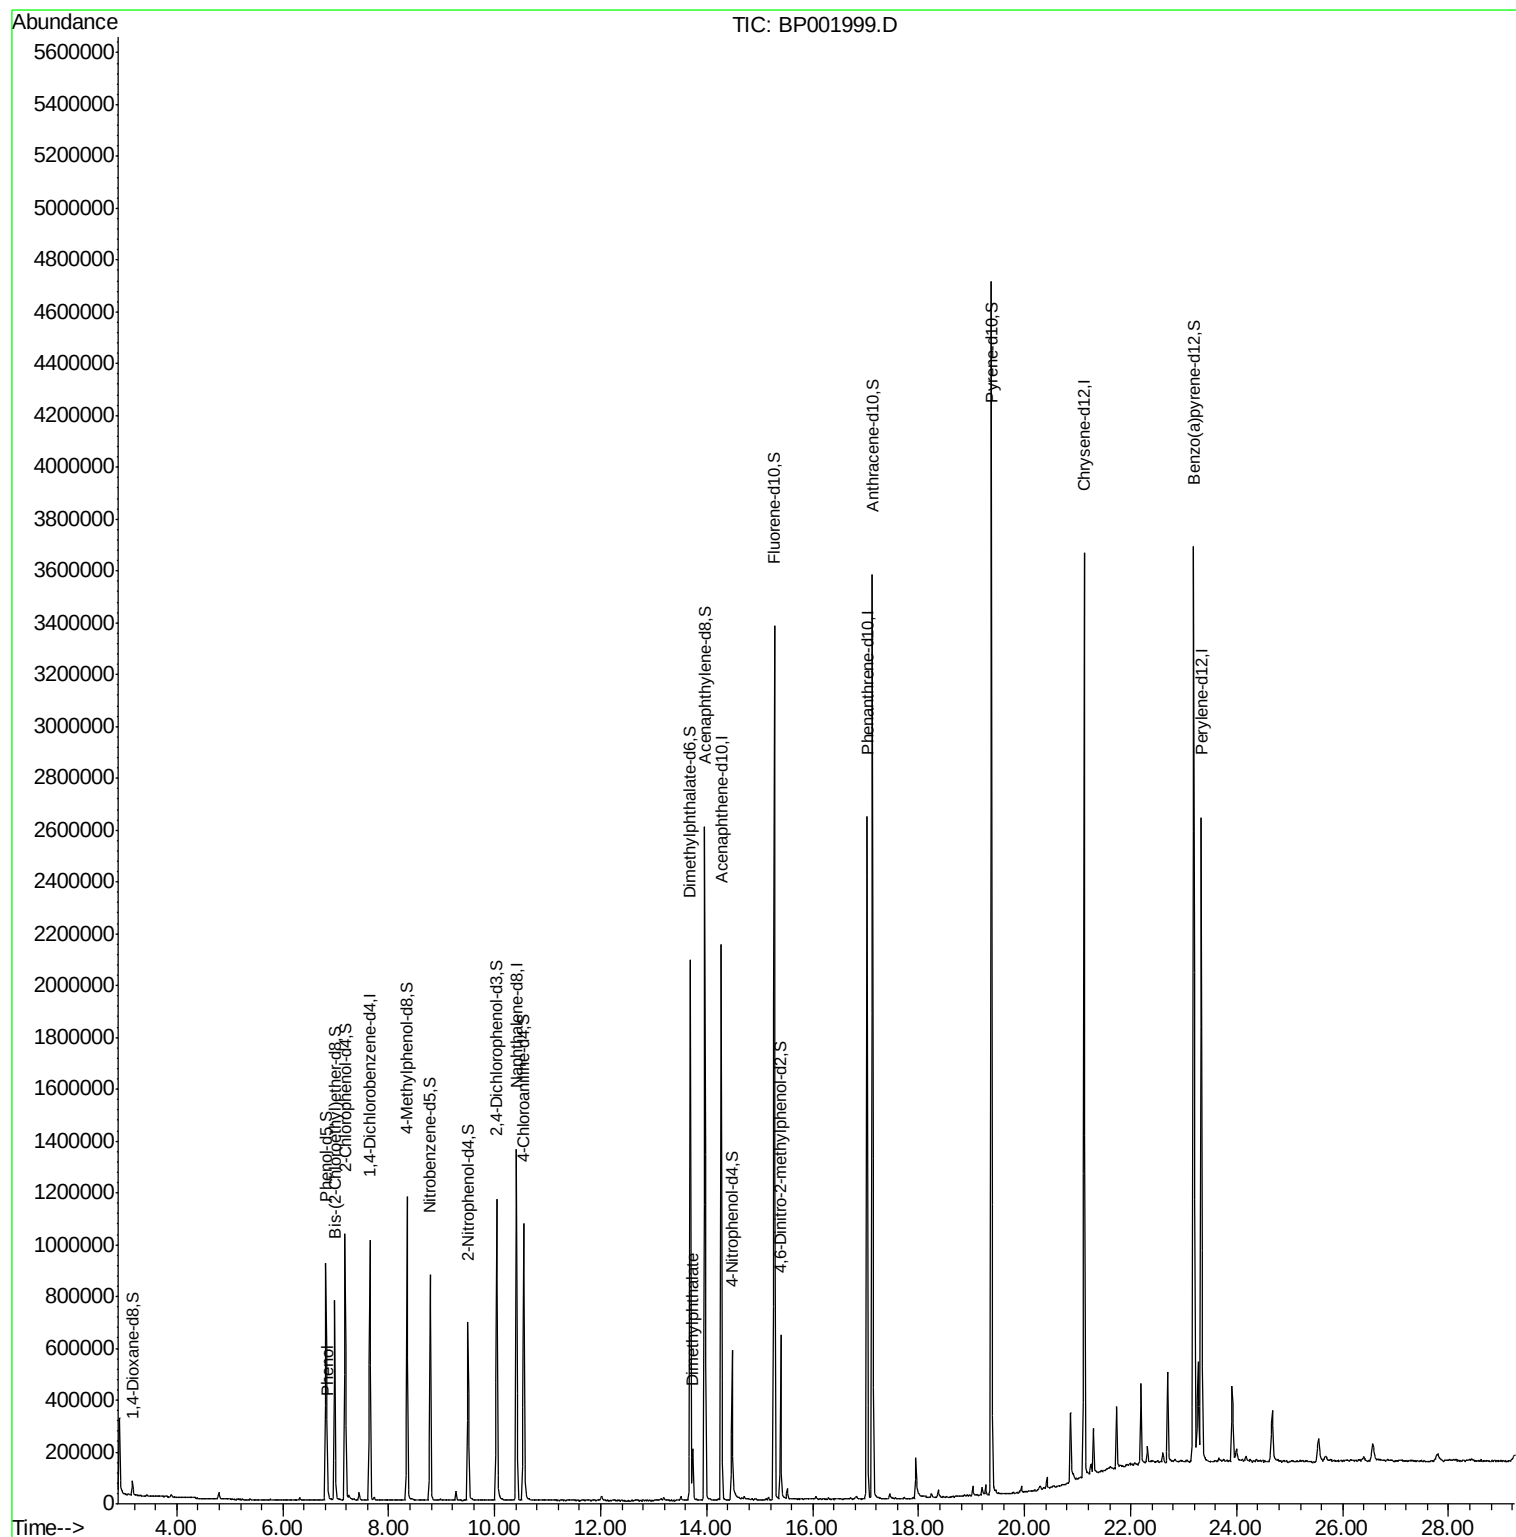

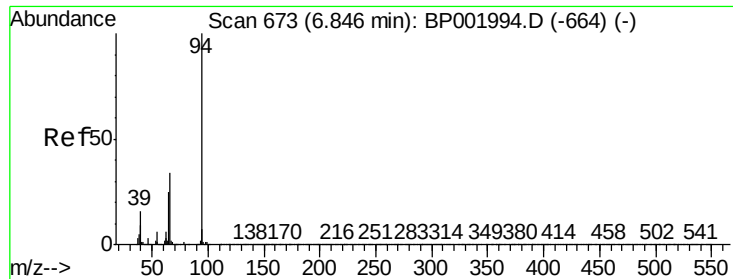

#6

Phenol

Concen: 1.298 ng/ul

RT: 6.85 min Scan# 673

Delta R.T. 0.00 min

Lab File: BP001999.D

Acq: 02 Mar 2020 20:24

Instrument :

BNA_P

ClientSampleId :

DBDQ1





Tot Ion: 94 Resp: 29261

Ion Ratio Lower Upper

94 100

65 29.3 20.6 30.8

66 37.9 28.2 42.2

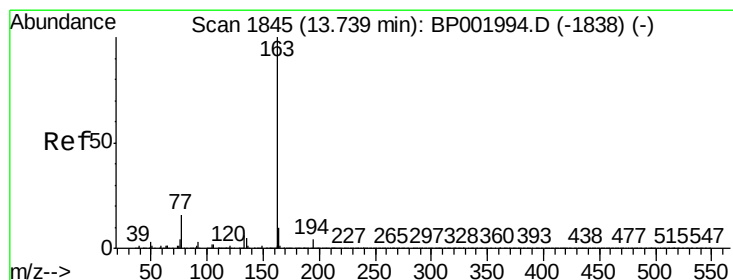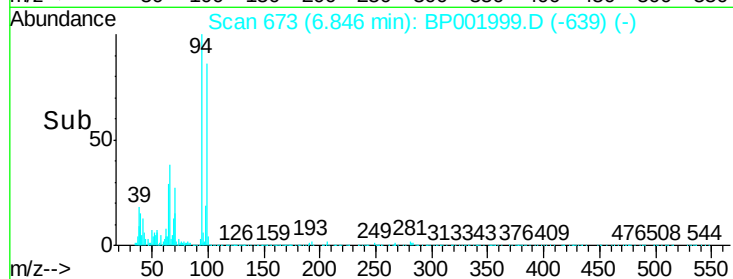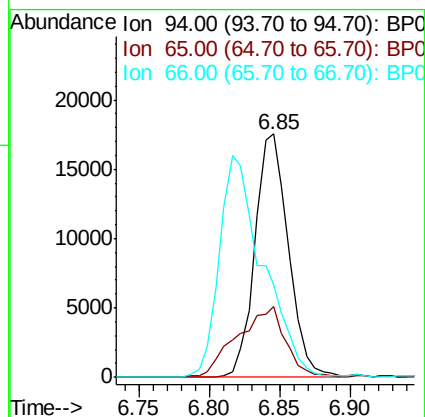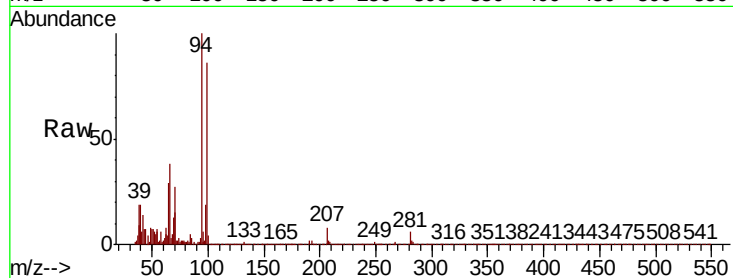

#45

Dimethylphthalate

Concen: 2.346 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BP001999.D

Acq: 02 Mar 2020 20:24

Tgt Ion: 163 Resp: 135028

Ion Ratio Lower Upper

163 100

194 4.8 3.6 5.4

164 10.3 8.2 12.4

