

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030220\
 Data File : BP002011.D
 Acq On : 03 Mar 2020 04:52
 Operator : CG/JU
 Sample : L1616-20
 Misc :
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBDR4

Quant Time: Mar 03 05:33:50 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 05:31:15 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	324297	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1329301	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	826495	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1761493	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1740828	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1999830	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.17	96	42704	5.66	ng/uL	0.00
5) Phenol-d5	6.82	99	758649	30.67	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	431594	32.95	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	672455	31.42	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	627129	30.85	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	317414	31.08	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	356013	30.99	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	660607	29.85	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	889333	36.66	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1922964	30.74	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2353908	31.47	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	261060	21.83	ng/ul	0.00
58) Fluorene-d10	15.27	176	1693333	31.29	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	203183	20.92	ng/ul	0.00
71) Anthracene-d10	17.13	188	2513298	31.75	ng/ul	0.00
79) Pyrene-d10	19.37	212	2871844	31.51	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	3221160	31.48	ng/ul	0.00

Target Compounds


					Ovalue
6) Phenol	6.85	94	34064	1.326	ng/ul 97
45) Dimethylphthalate	13.73	163	177858	2.755	ng/ul 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030220\
Data File : BP002011.D
Acq On : 03 Mar 2020 04:52
Operator : CG/JU
Sample : L1616-20
Misc :
ALS Vial : 30 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBDR4

Quant Time: Mar 03 05:33:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 05:31:15 2020
Response via : Initial Calibration

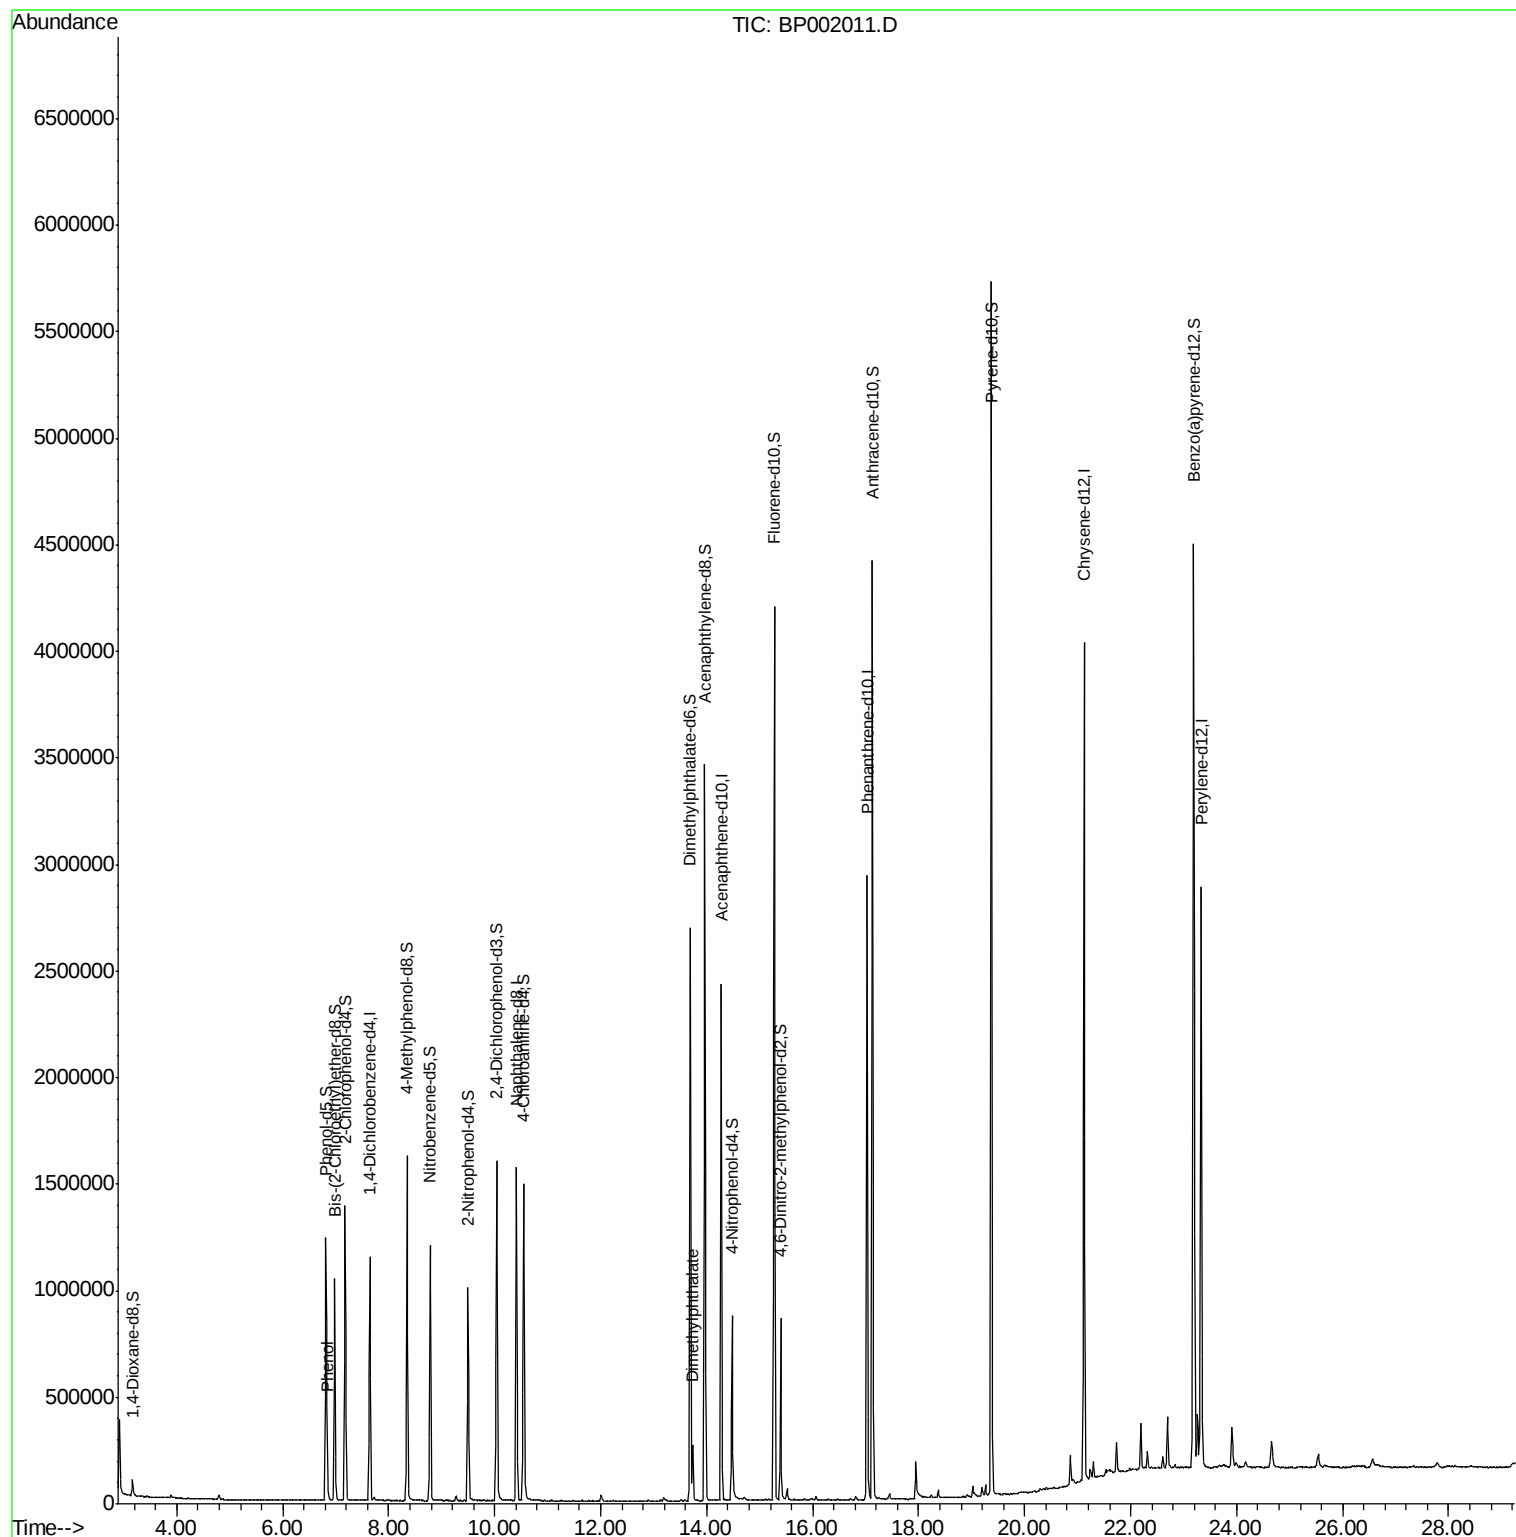

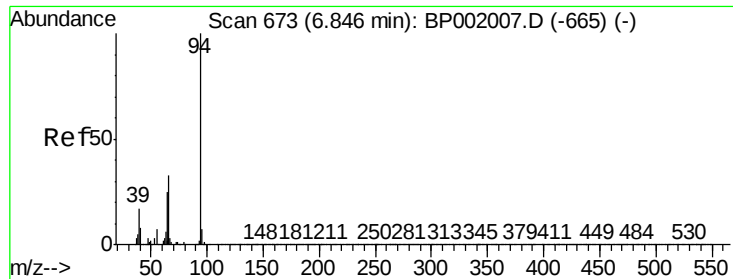





#6

Phenol

Concen: 1.326 ng/ul
 RT: 6.85 min Scan# 673
 Delta R.T. -0.00 min
 Lab File: BP002011.D
 Acq: 03 Mar 2020 04:52

Instrument :
 BNA_P
 ClientSampleId :
 DBDR4

Tot Ion: 94 Resp: 34064
 Ion Ratio Lower Upper
 94 100
 65 25.2 20.6 30.8
 66 37.3 28.2 42.2

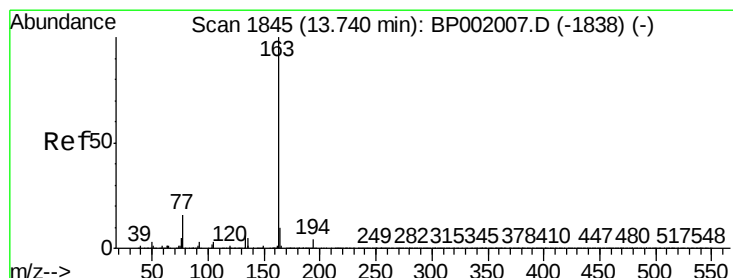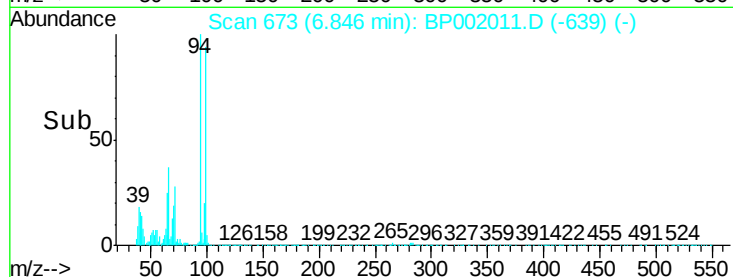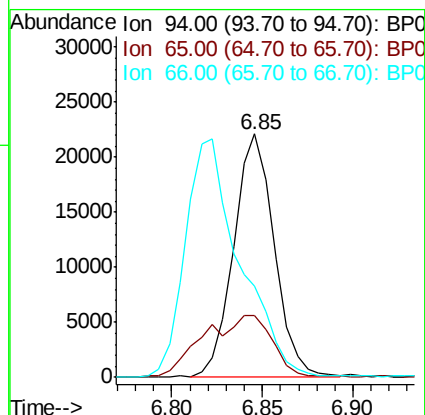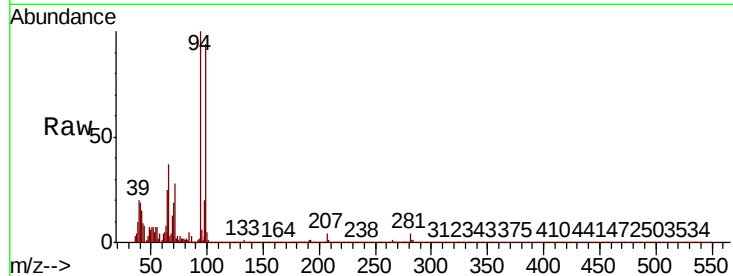

#45

Dimethylphthalate

Concen: 2.755 ng/ul
 RT: 13.73 min Scan# 1844
 Delta R.T. -0.01 min
 Lab File: BP002011.D
 Acq: 03 Mar 2020 04:52

Tgt Ion: 163 Resp: 177858
 Ion Ratio Lower Upper
 163 100
 194 4.6 3.6 5.4
 164 10.6 8.2 12.4

