

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030220\
 Data File : BP002024.D
 Acq On : 03 Mar 2020 16:45
 Operator : CG/JU
 Sample : L1617-07
 Misc :
 ALS Vial : 42 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBDS1

Quant Time: Mar 04 06:16:40 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 05:31:15 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	293075	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1239525	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	780362	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1715176	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1674382	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1873606	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.17	96	36082	5.29	ng/uL	0.00
5) Phenol-d5	6.82	99	660321	29.54	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	371534	31.38	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	582051	30.10	ng/ul	0.00
13) 4-Methylphenol-d8	8.34	113	542486	29.53	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	277988	29.20	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	309804	28.92	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	588966	28.54	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	759043	33.55	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1706095	28.89	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2115330	29.95	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	216702	19.19	ng/ul	0.00
58) Fluorene-d10	15.27	176	1536943	30.08	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	165683	17.52	ng/ul	0.00
71) Anthracene-d10	17.13	188	2311185	29.98	ng/ul	0.00
79) Pyrene-d10	19.37	212	2588522	29.53	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	2888368	30.13	ng/ul	0.00
Target Compounds						
6) Phenol	6.84	94	26872	1.158	ng/ul	92
45) Dimethylphthalate	13.73	163	209890	3.443	ng/ul	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030220\
Data File : BP002024.D
Acq On : 03 Mar 2020 16:45
Operator : CG/JU
Sample : L1617-07
Misc :
ALS Vial : 42 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBDS1

Quant Time: Mar 04 06:16:40 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 05:31:15 2020
Response via : Initial Calibration

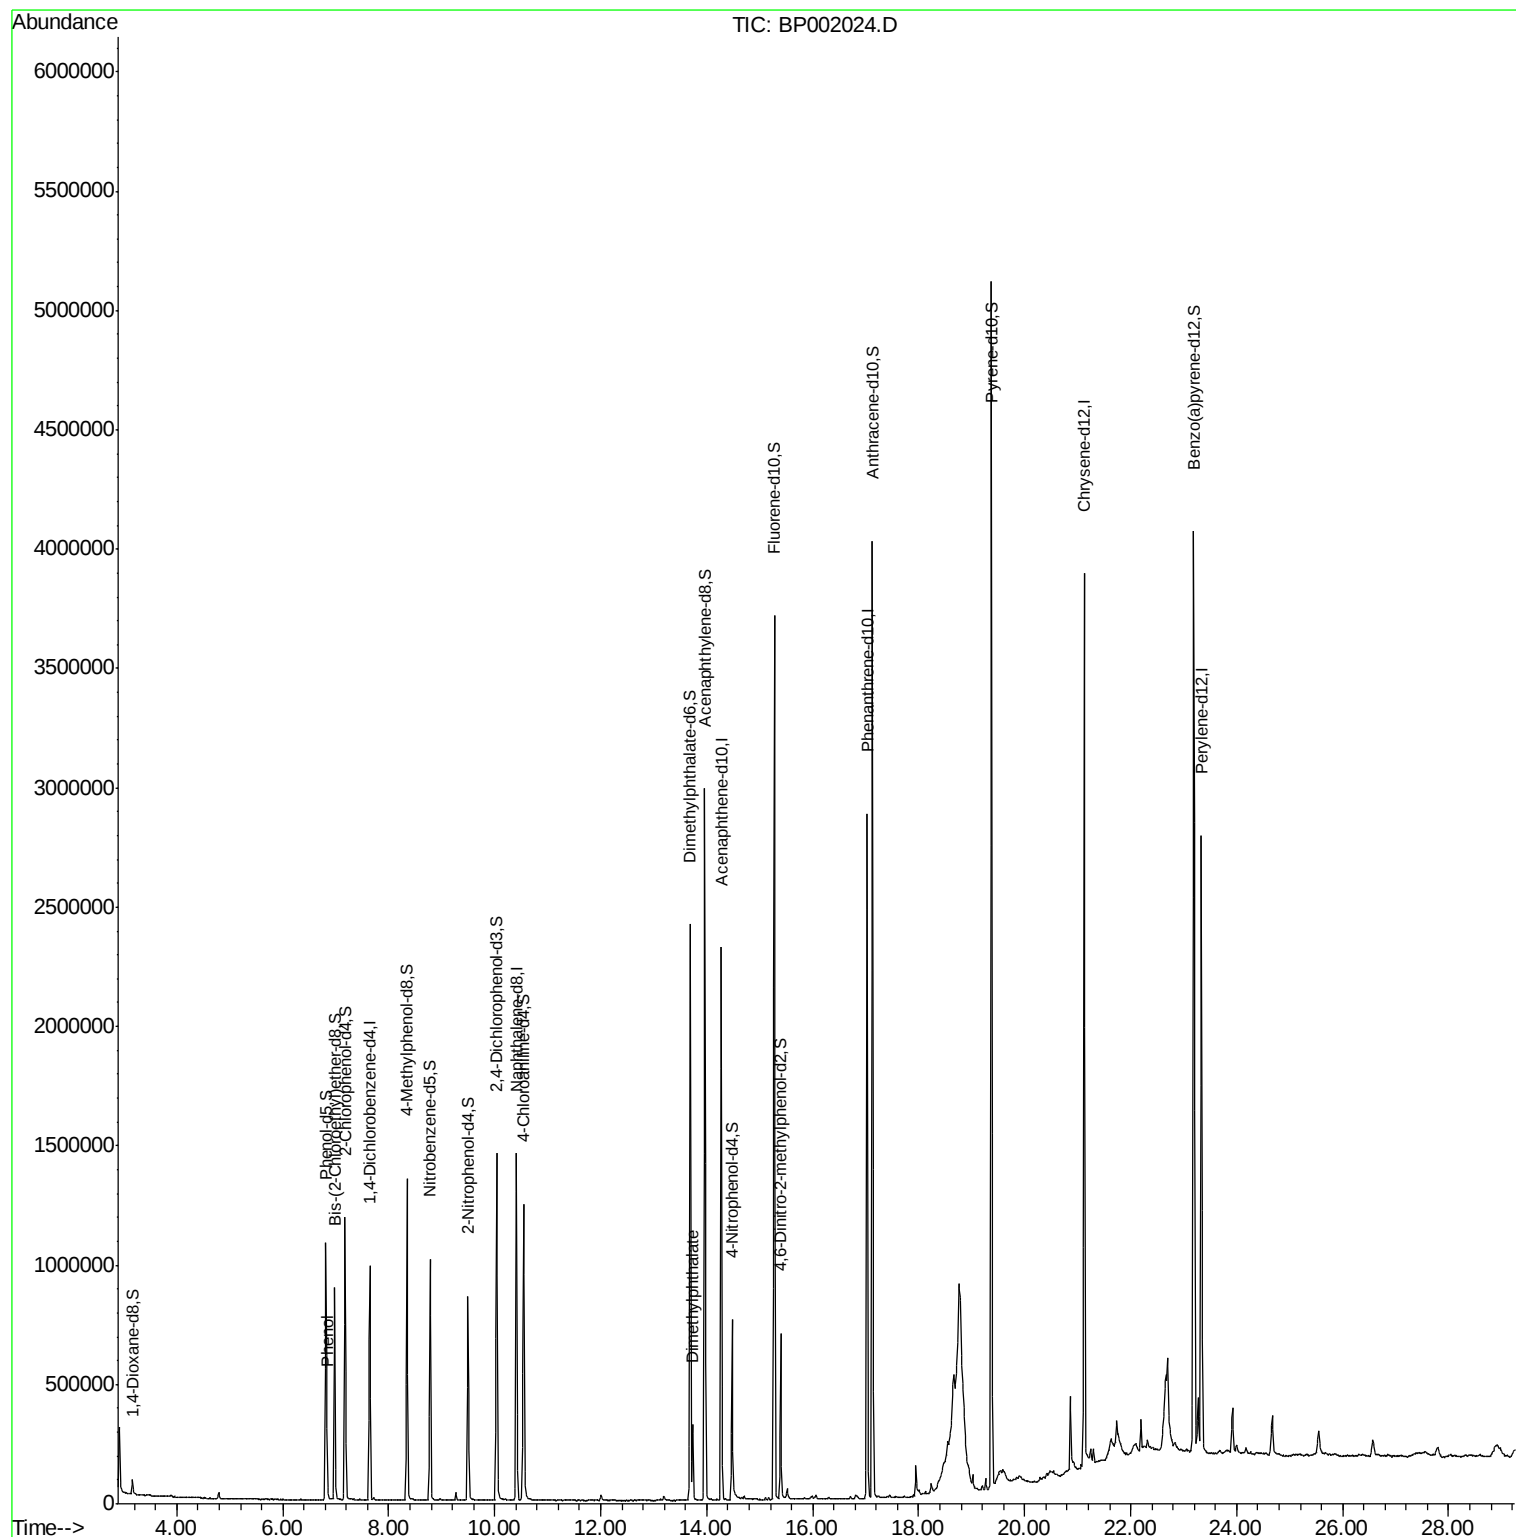

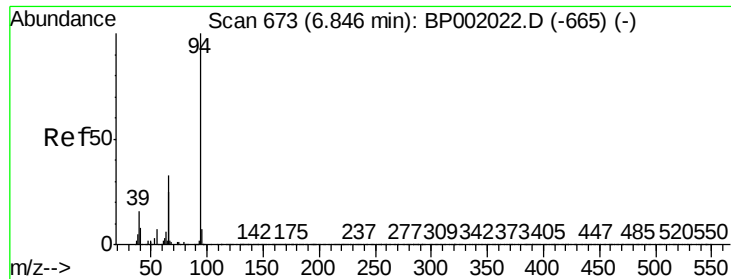

#6

Phenol

Concen: 1.158 ng/ul

RT: 6.84 min Scan# 672

Delta R.T. -0.01 min

Lab File: BP002024.D

Acq: 03 Mar 2020 16:45

Instrument :

BNA_P

ClientSampleId :

DBDS1


Tot Ion: 94 Resp: 26872

Ion Ratio Lower Upper

94 100

65 29.7 20.6 30.8




66 39.6 28.2 42.2

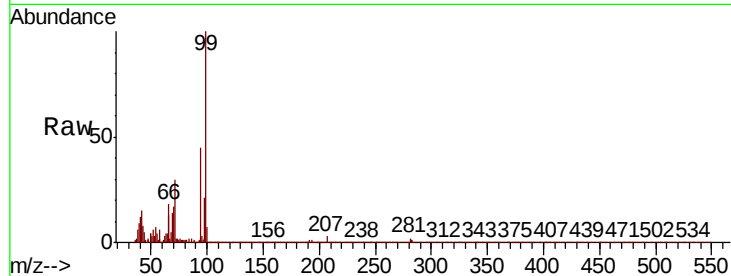

Abundance Ion 94.00 (93.70 to 94.70): BP0

Ion 65.00 (64.70 to 65.70): BP0

Ion 66.00 (65.70 to 66.70): BP0

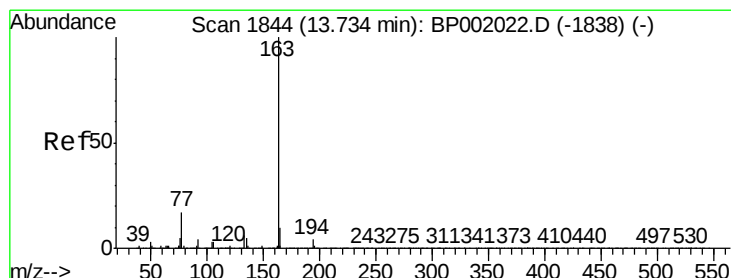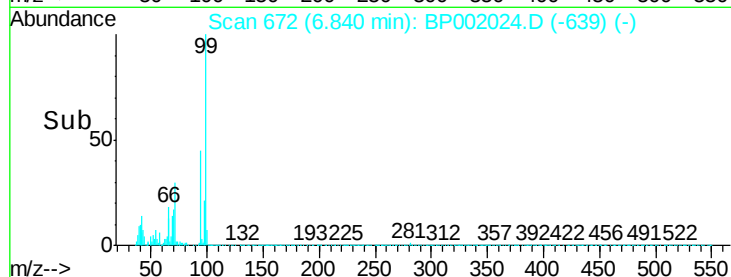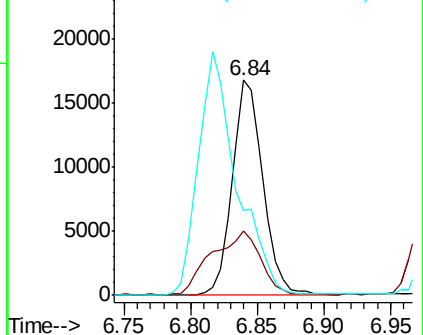

#45

Dimethylphthalate

Concen: 3.443 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BP002024.D

Acq: 03 Mar 2020 16:45


Tgt Ion: 163 Resp: 209890

Ion Ratio Lower Upper

163 100

194 4.4 3.6 5.4

164 10.4 8.2 12.4

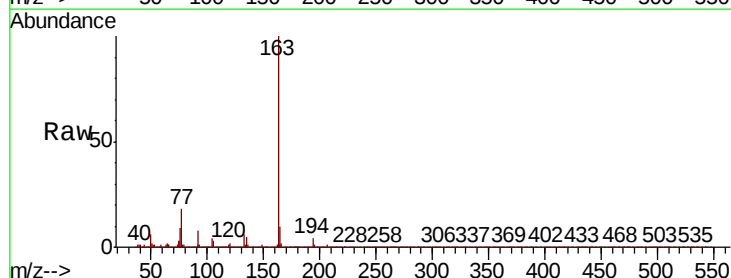

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

