

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030220\
 Data File : BP002028.D
 Acq On : 03 Mar 2020 19:01
 Operator : CG/JU
 Sample : L1617-10
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBDS4

Quant Time: Mar 04 05:15:03 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 05:31:15 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	311043	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1301973	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	839103	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1801720	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1739421	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1955638	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.17	96	19572	2.71	ng/uL	0.00
5) Phenol-d5	6.82	99	373067	15.72	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	218959	17.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	324767	15.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	297472	15.26	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	154006	15.40	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	164973	14.66	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	330968	15.27	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	386086	16.25	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1137054	17.91	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	1279110	16.84	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	114758	9.45	ng/ul	0.00
58) Fluorene-d10	15.27	176	980350	17.84	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	91442	9.21	ng/ul	0.00
71) Anthracene-d10	17.13	188	1547601	19.11	ng/ul	0.00
79) Pyrene-d10	19.37	212	1799655	19.76	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	1906393	19.05	ng/ul	0.00


Target Compounds					Ovalue	
6) Phenol	6.85	94	24654	1.001	ng/ul	96
45) Dimethylphthalate	13.73	163	142903	2.180	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030220\
Data File : BP002028.D
Acq On : 03 Mar 2020 19:01
Operator : CG/JU
Sample : L1617-10
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBDS4

Quant Time: Mar 04 05:15:03 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 05:31:15 2020
Response via : Initial Calibration

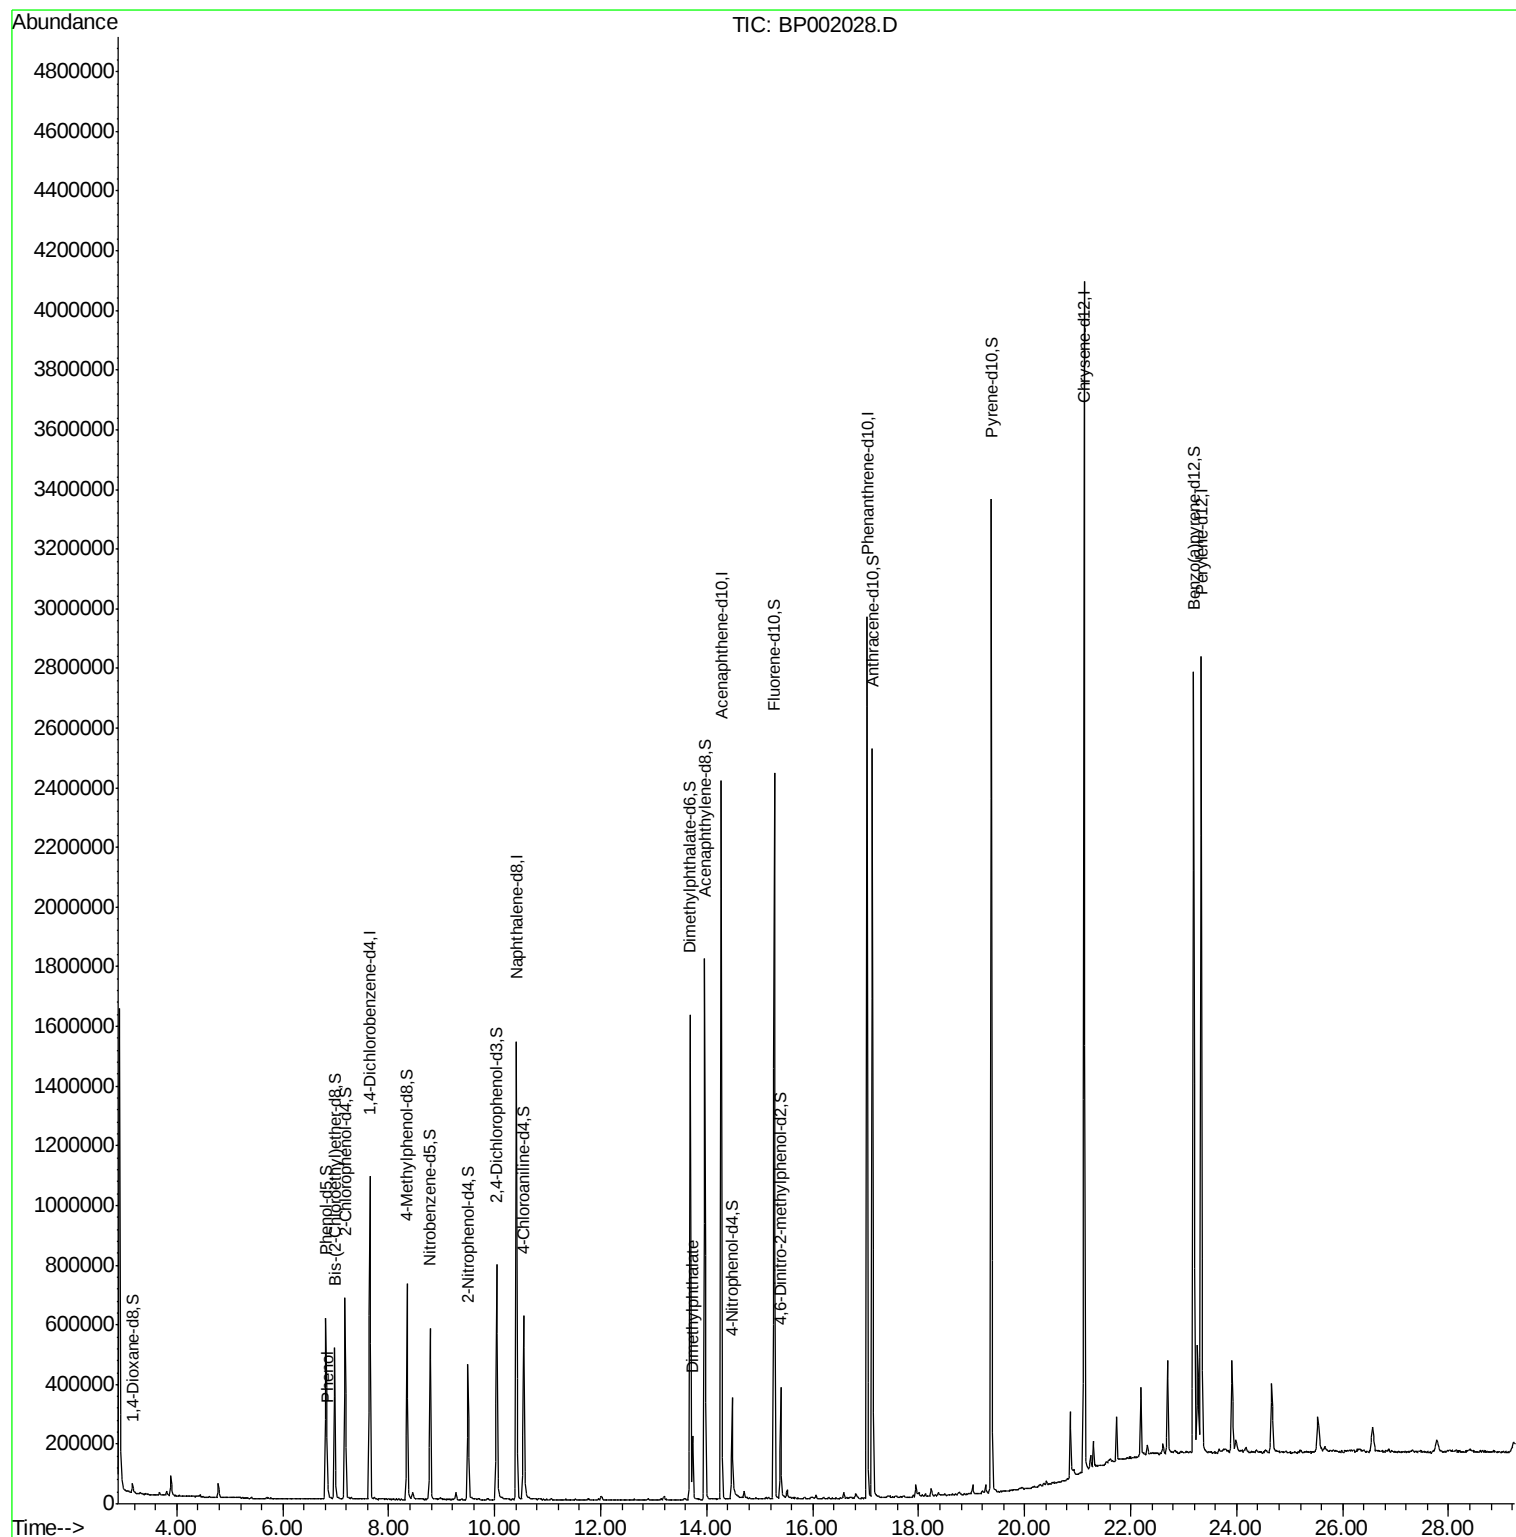

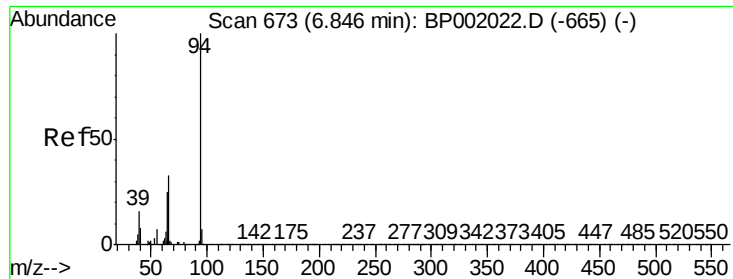

#6

Phenol

Concen: 1.001 ng/ul

RT: 6.85 min Scan# 673

Delta R.T. -0.00 min

Lab File: BP002028.D

Acq: 03 Mar 2020 19:01

Instrument :

BNA_P

ClientSampleId :

DBDS4





Tot Ion: 94 Resp: 24654

Ion Ratio Lower Upper

94 100

65 25.4 20.6 30.8

66 38.9 28.2 42.2

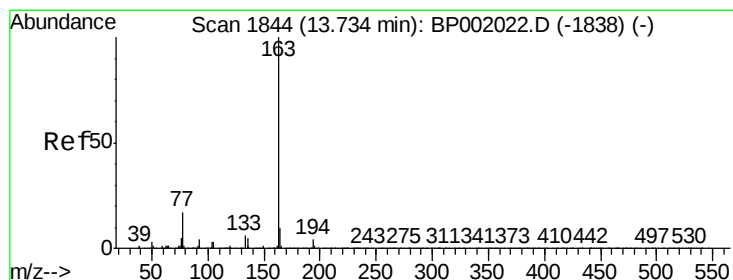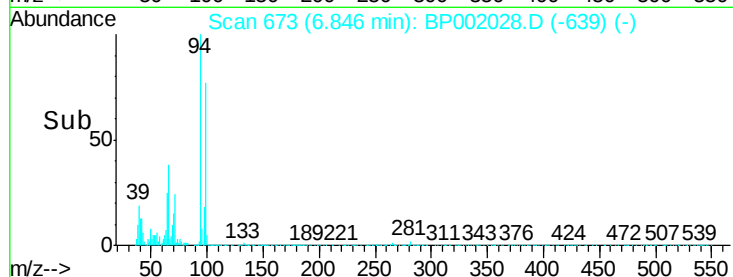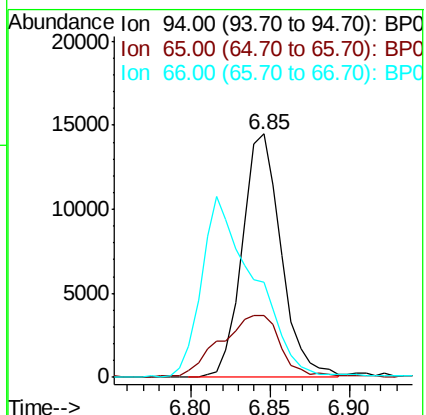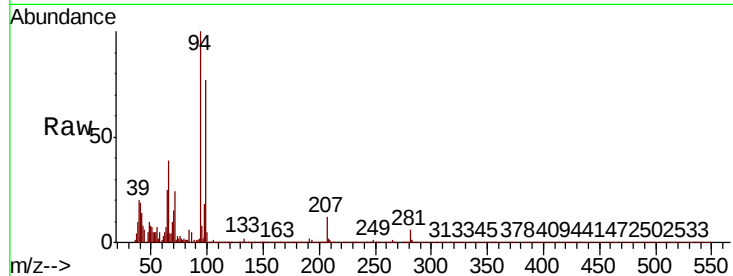

#45

Dimethylphthalate

Concen: 2.180 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BP002028.D

Acq: 03 Mar 2020 19:01

Tgt Ion: 163 Resp: 142903

Ion Ratio Lower Upper

163 100

194 4.2 3.6 5.4

164 10.5 8.2 12.4

