

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030220\
 Data File : BP002034.D
 Acq On : 03 Mar 2020 23:33
 Operator : CG/JU
 Sample : L1617-16
 Misc :
 ALS Vial : 53 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DBDT0

Quant Time: Mar 04 05:16:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 05:31:15 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	322375	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1347156	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	877794	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1902282	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1873949	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	2051793	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.17	96	38965	5.20	ng/uL	0.00
5) Phenol-d5	6.82	99	662362	26.94	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	393639	30.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	598178	28.12	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	475637	23.54	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	279662	27.02	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	302344	25.97	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.03	165	587421	26.19	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	622185	25.31	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	1803358	27.15	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	2196752	27.65	ng/ul	0.00
52) 4-Nitrophenol-d4	14.47	143	212757	16.75	ng/ul	0.00
58) Fluorene-d10	15.27	176	1633091	28.41	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	149150	14.22	ng/ul	0.00
71) Anthracene-d10	17.13	188	2443898	28.58	ng/ul	0.00
79) Pyrene-d10	19.37	212	2795108	28.49	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	2986733	28.45	ng/ul	0.00

Target Compounds


				Ovalue	
6) Phenol	6.85	94	28299	1.109	ng/ul 96
45) Dimethylphthalate	13.73	163	218894	3.192	ng/ul 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030220\
Data File : BP002034.D
Acq On : 03 Mar 2020 23:33
Operator : CG/JU
Sample : L1617-16
Misc :
ALS Vial : 53 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DBDT0

Quant Time: Mar 04 05:16:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 05:31:15 2020
Response via : Initial Calibration

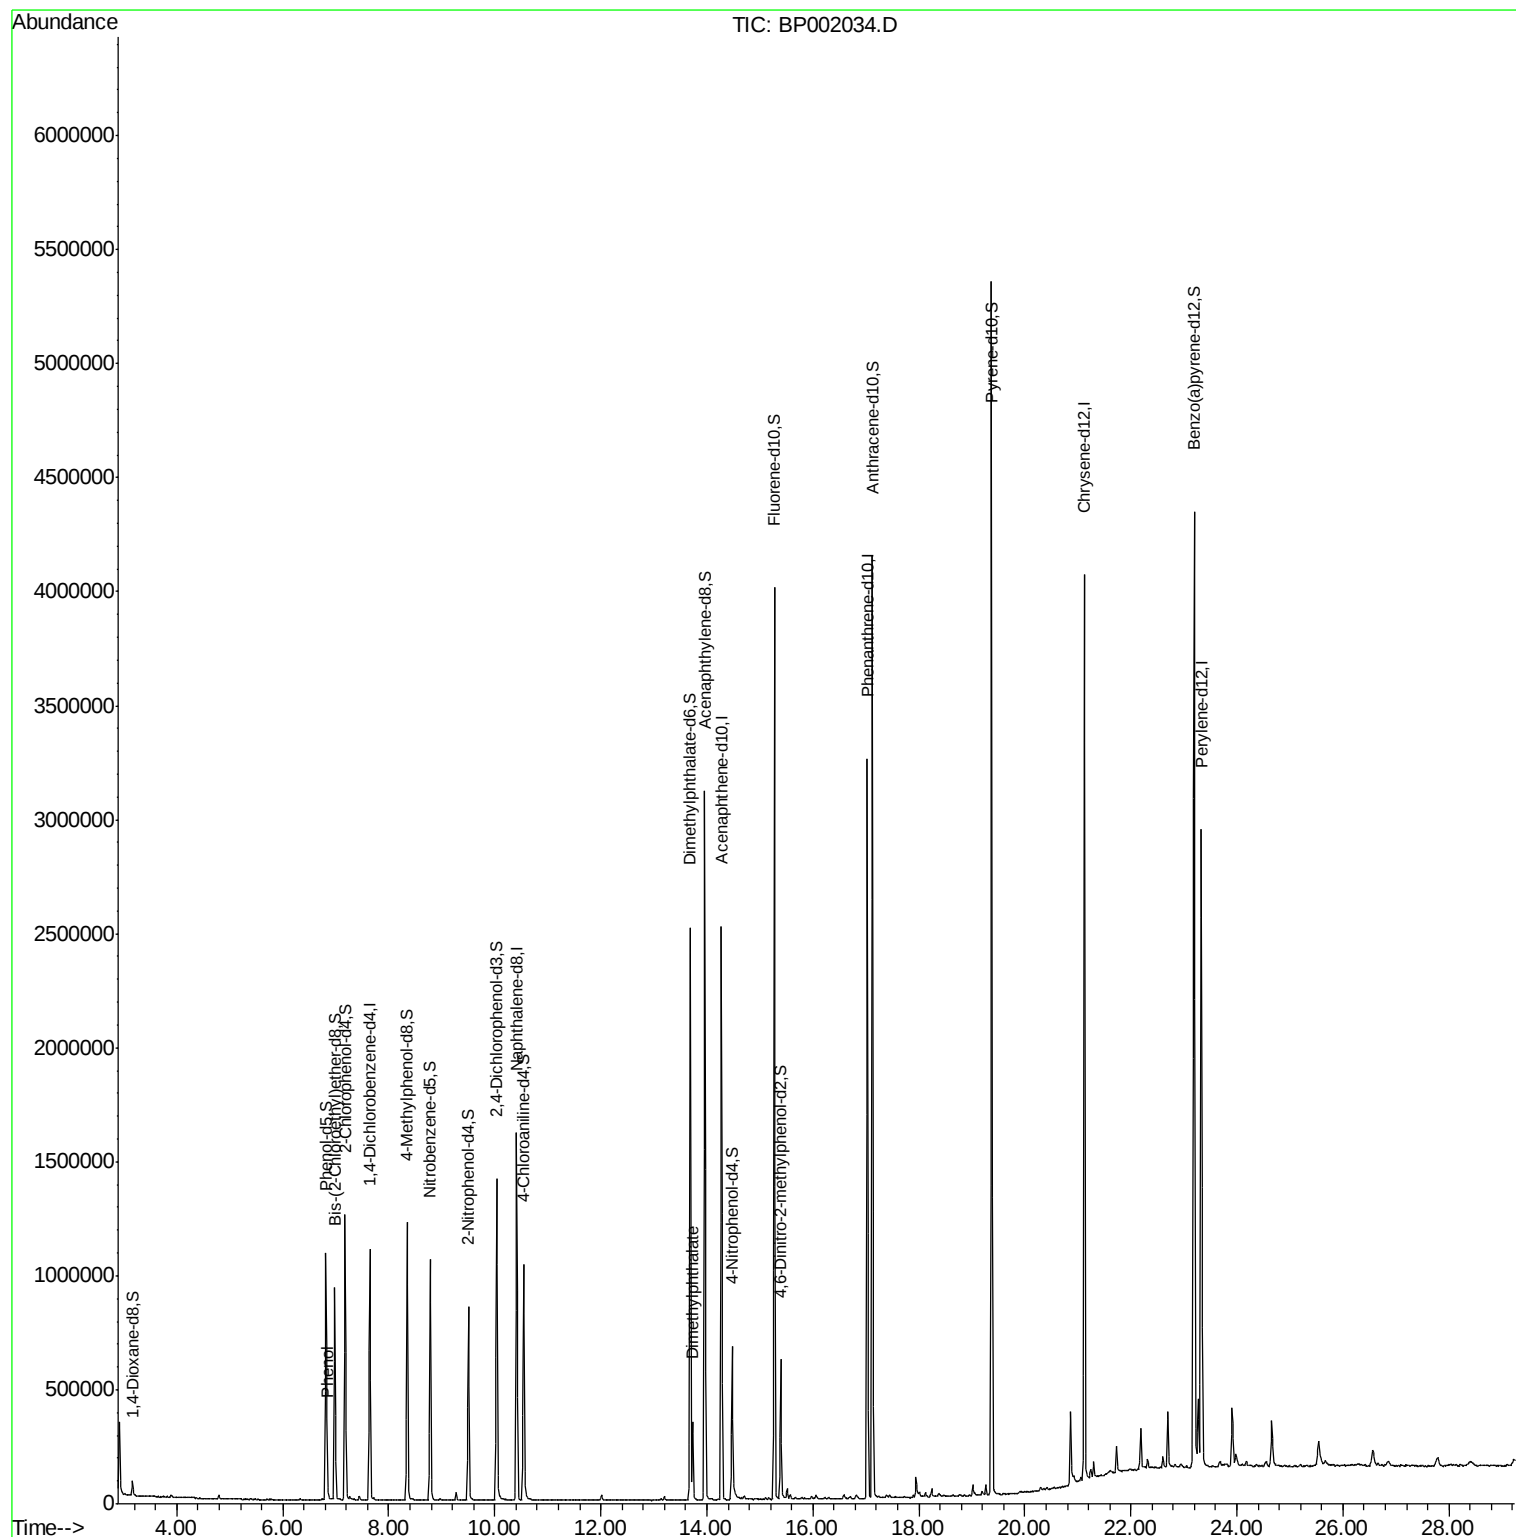

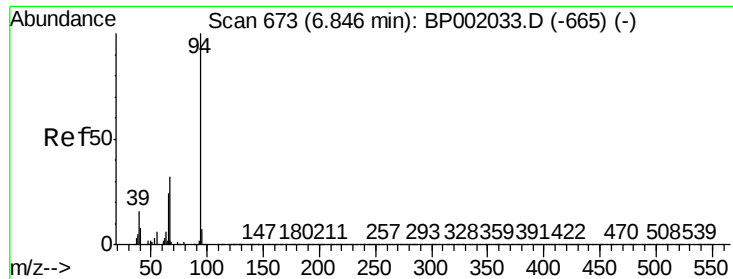

#6

Phenol

Concen: 1.109 ng/ul

RT: 6.85 min Scan# 673

Delta R.T. 0.00 min

Lab File: BP002034.D

Acq: 03 Mar 2020 23:33

Instrument :

BNA_P

ClientSampleId :

DBDT0





Tot Ion: 94 Resp: 28299

Ion Ratio Lower Upper

94 100

65 26.1 20.6 30.8

66 38.6 28.2 42.2

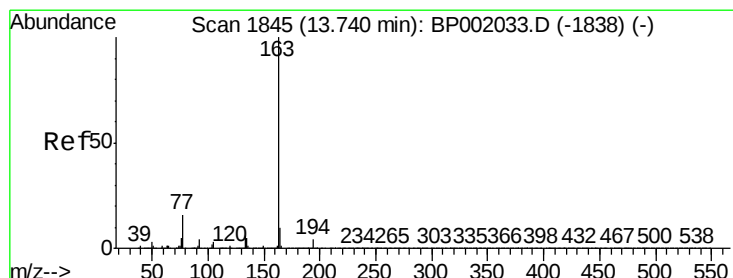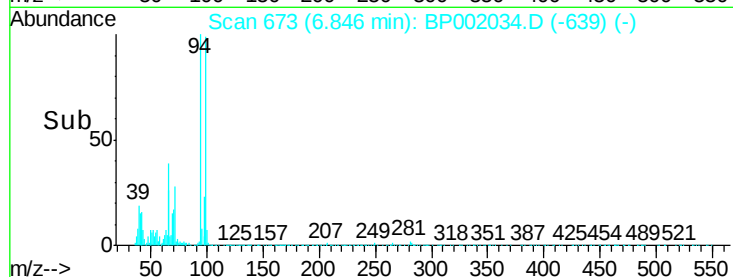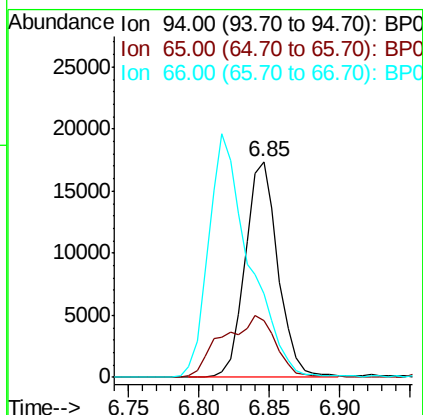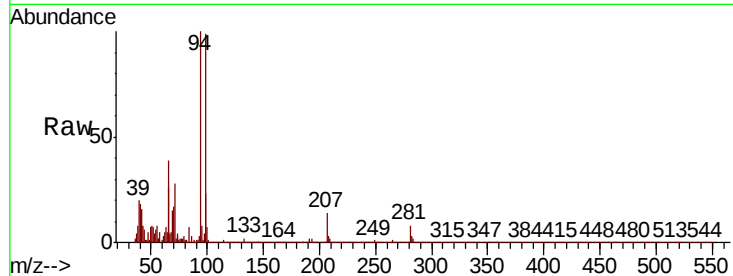

#45

Dimethylphthalate

Concen: 3.192 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BP002034.D

Acq: 03 Mar 2020 23:33

Tgt Ion: 163 Resp: 218894

Ion Ratio Lower Upper

163 100

194 4.3 3.6 5.4

164 10.2 8.2 12.4

