
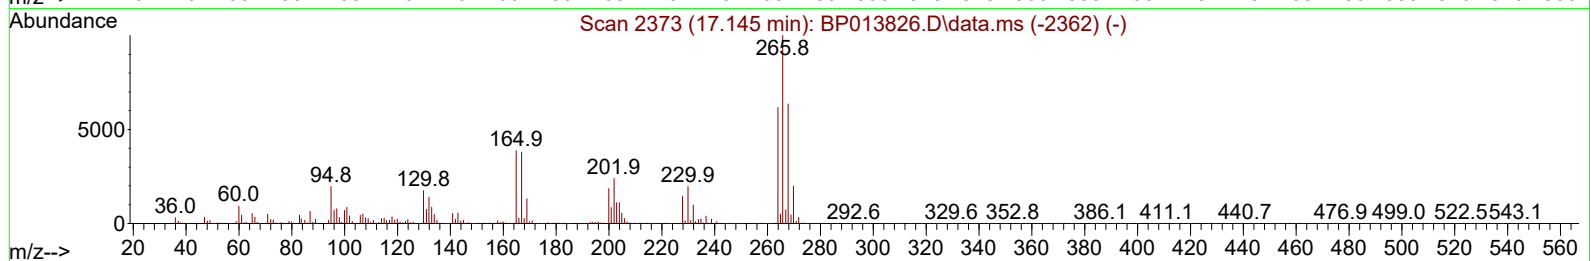
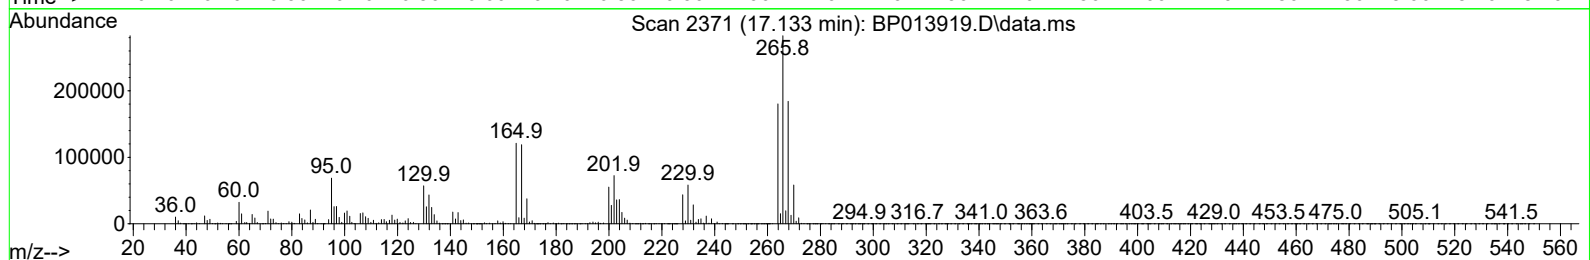


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030223\
Data File : BP013919.D
Acq On : 02 Mar 2023 13:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 05:51:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 02 04:26:35 2023
Response via : Initial Calibration

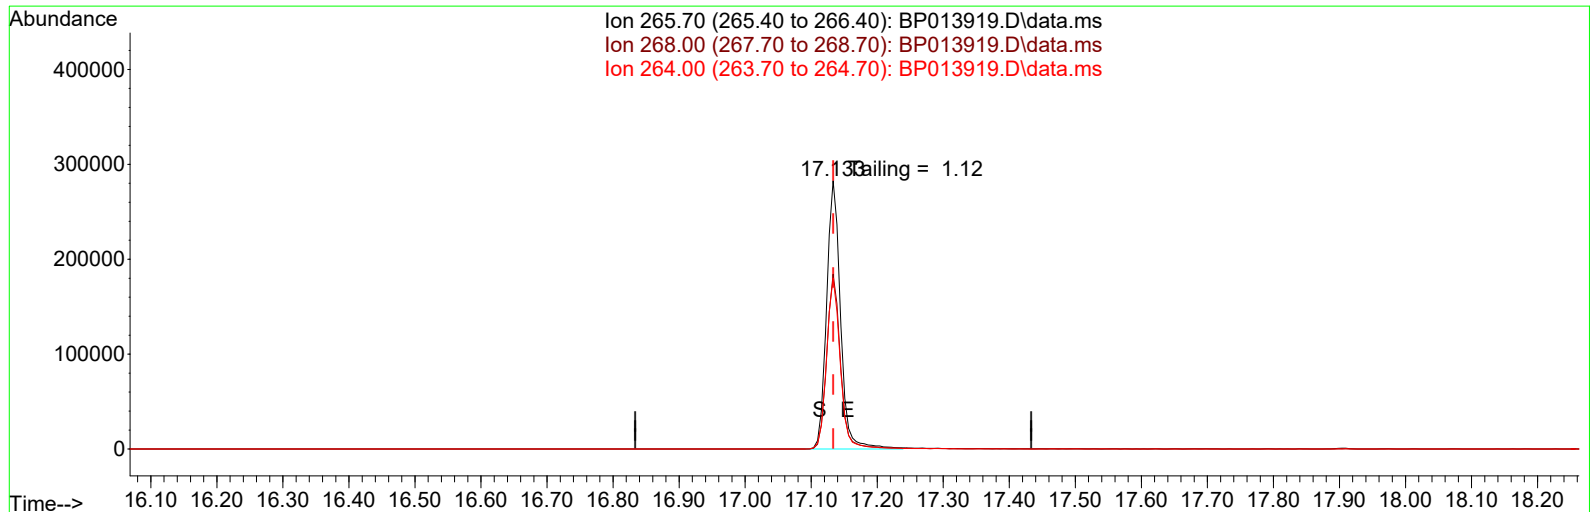

TIC: BP013919.D\data.ms

(70) Pentachlorophenol (C)




17.133min (-0.000) 1755427.03 ng

response 416876

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	65.13
264.00	61.70	63.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030223\
Data File : BP013919.D
Acq On : 02 Mar 2023 13:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 03 05:51:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 02 04:26:35 2023
Response via : Initial Calibration

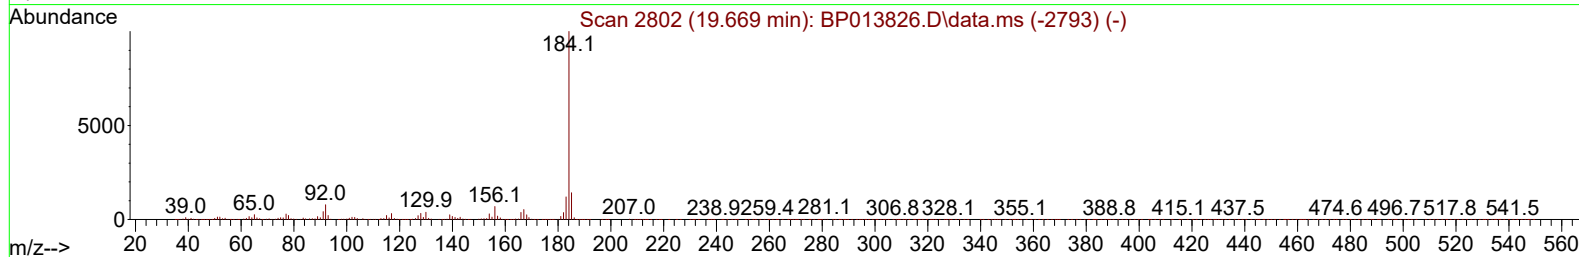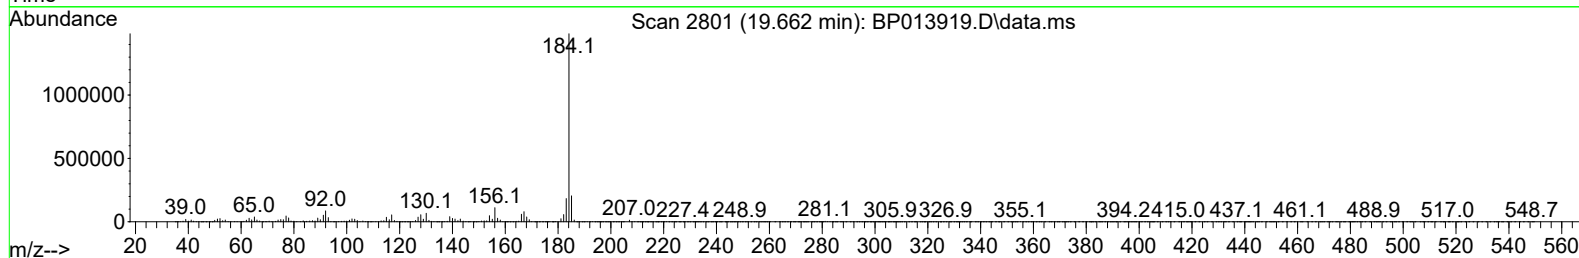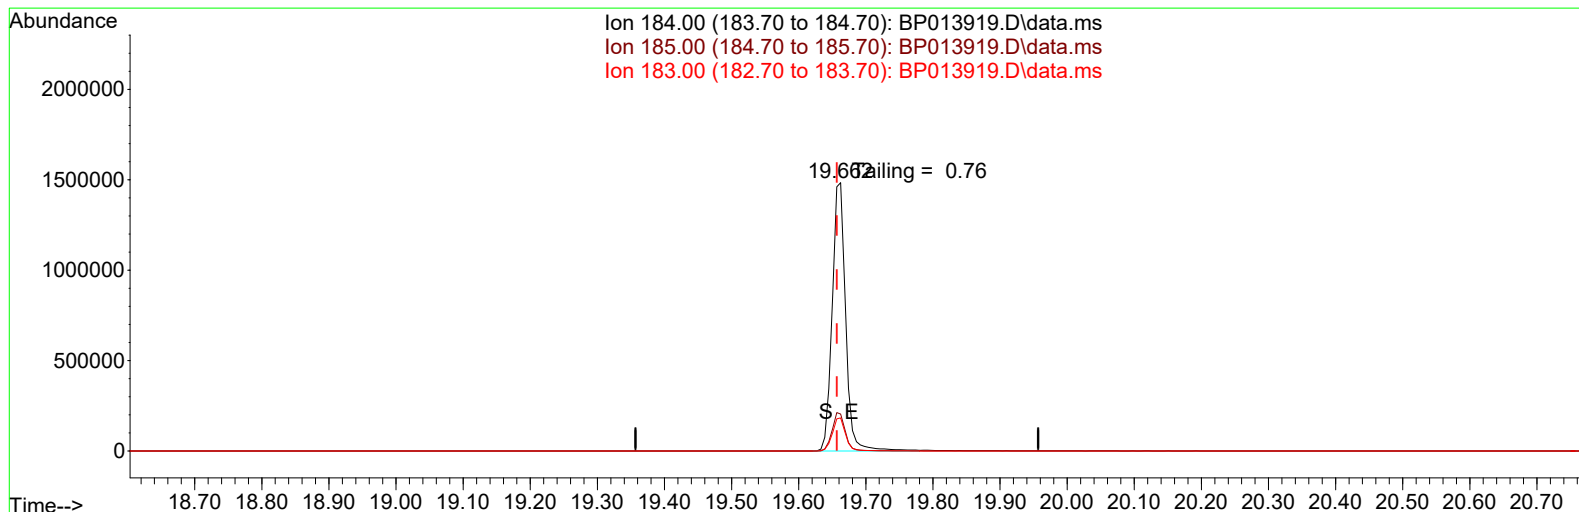

TIC: BP013919.D\data.ms

(77) Benzidine**19.662min (+ 0.006) 1437780.56 ng****response 2066939**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.76
183.00	12.00	12.37
0.00	0.00	0.00