

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030223\
 Data File : BP013924.D
 Acq On : 02 Mar 2023 16:15
 Operator : CG/JU
 Sample : 01739-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SAMPLE-1-COMP-1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP013924.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.487	47	51	56	rVB	156696	170709	2.38%	0.568%
2	5.128	324	330	332	rBV	80670	109071	1.52%	0.363%
3	5.164	332	336	345	rVB	797149	1104728	15.43%	3.675%
4	5.634	409	416	429	rBV	1759264	2549946	35.61%	8.482%
5	7.246	683	690	713	rBV	1460811	2358880	32.94%	7.846%
6	8.093	827	834	846	rBV	343640	541669	7.56%	1.802%
7	9.269	1026	1034	1046	rBV	1018730	1714847	23.95%	5.704%
8	10.916	1307	1314	1327	rBV	421251	733900	10.25%	2.441%
9	13.357	1721	1729	1744	rBV	2707034	4071744	56.86%	13.544%
10	14.734	1955	1963	1972	rBV	675463	1043608	14.57%	3.471%
11	16.222	2209	2216	2236	rBV	2418400	3705623	51.75%	12.326%
12	17.487	2424	2431	2443	rBV	910718	1349349	18.84%	4.488%
13	20.022	2856	2862	2869	rBV	6070495	7161198	100.00%	23.820%
14	21.563	3119	3124	3132	rBV	1169377	1677719	23.43%	5.581%
15	24.116	3551	3558	3572	rVB2	834895	1770196	24.72%	5.888%




Sum of corrected areas: 30063187

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030223\
Data File : BP013924.D
Acq On : 02 Mar 2023 16:15
Operator : CG/JU
Sample : 01739-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SAMPLE-1-COMP-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

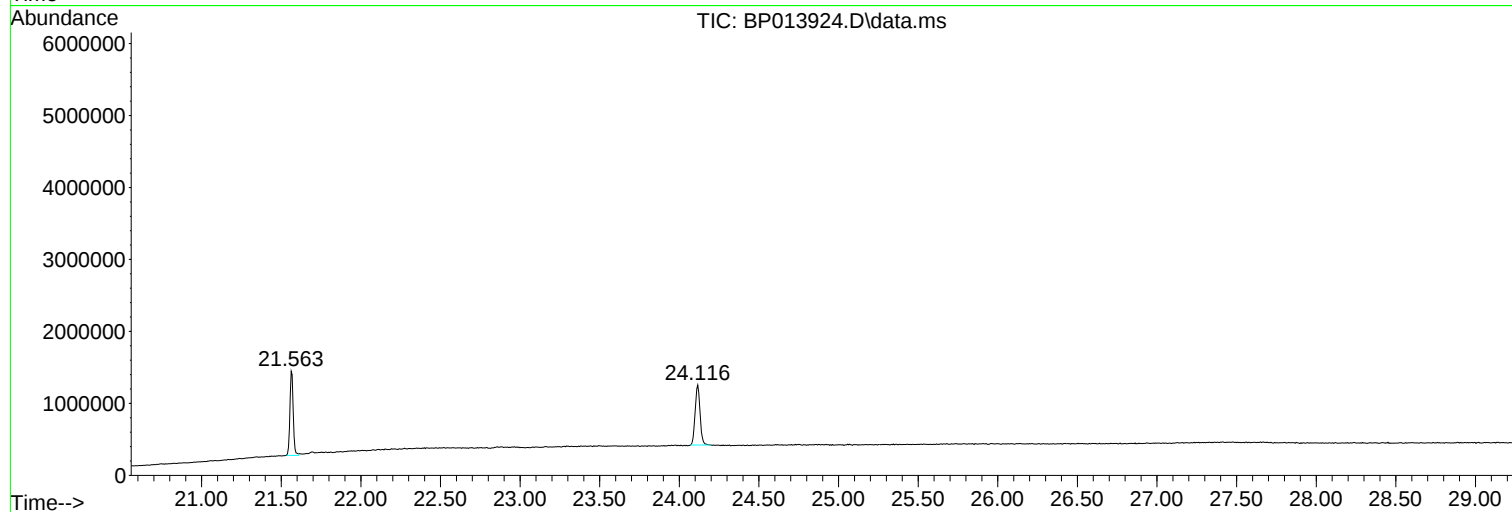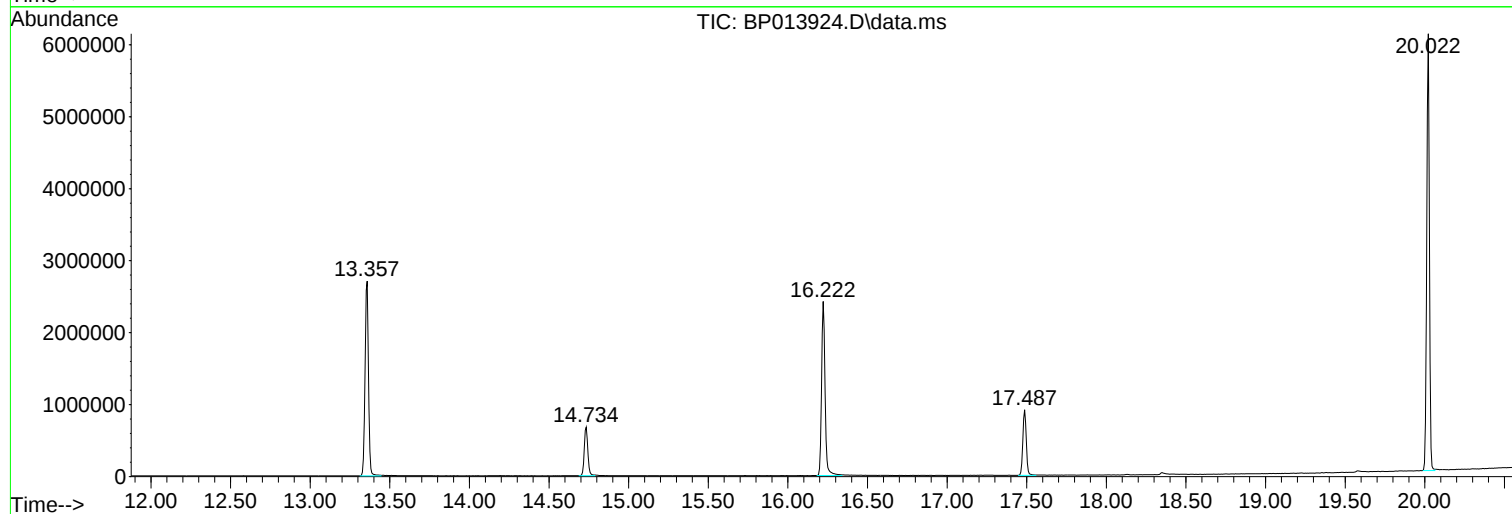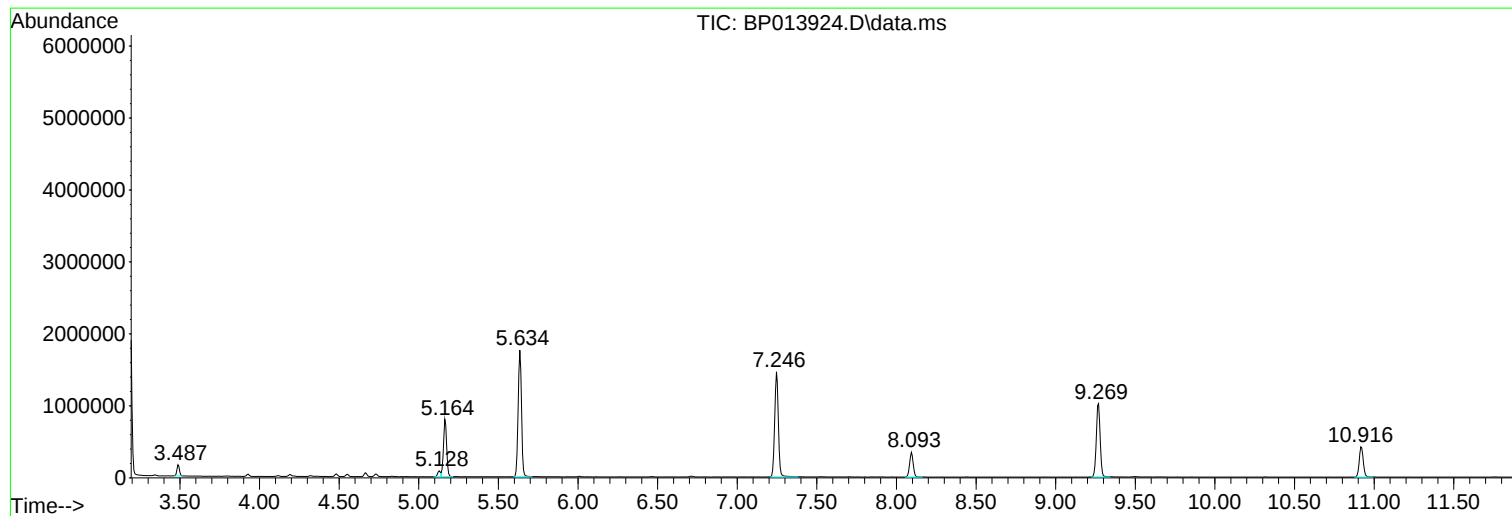

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030223\
Data File : BP013924.D
Acq On : 02 Mar 2023 16:15
Operator : CG/JU
Sample : 01739-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SAMPLE-1-COMP-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030223\
Data File : BP013924.D
Acq On : 02 Mar 2023 16:15
Operator : CG/JU
Sample : 01739-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SAMPLE-1-COMP-1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------