


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030223\
Data File : BP013919.D
Acq On : 02 Mar 2023 13:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 02 04:26:35 2023

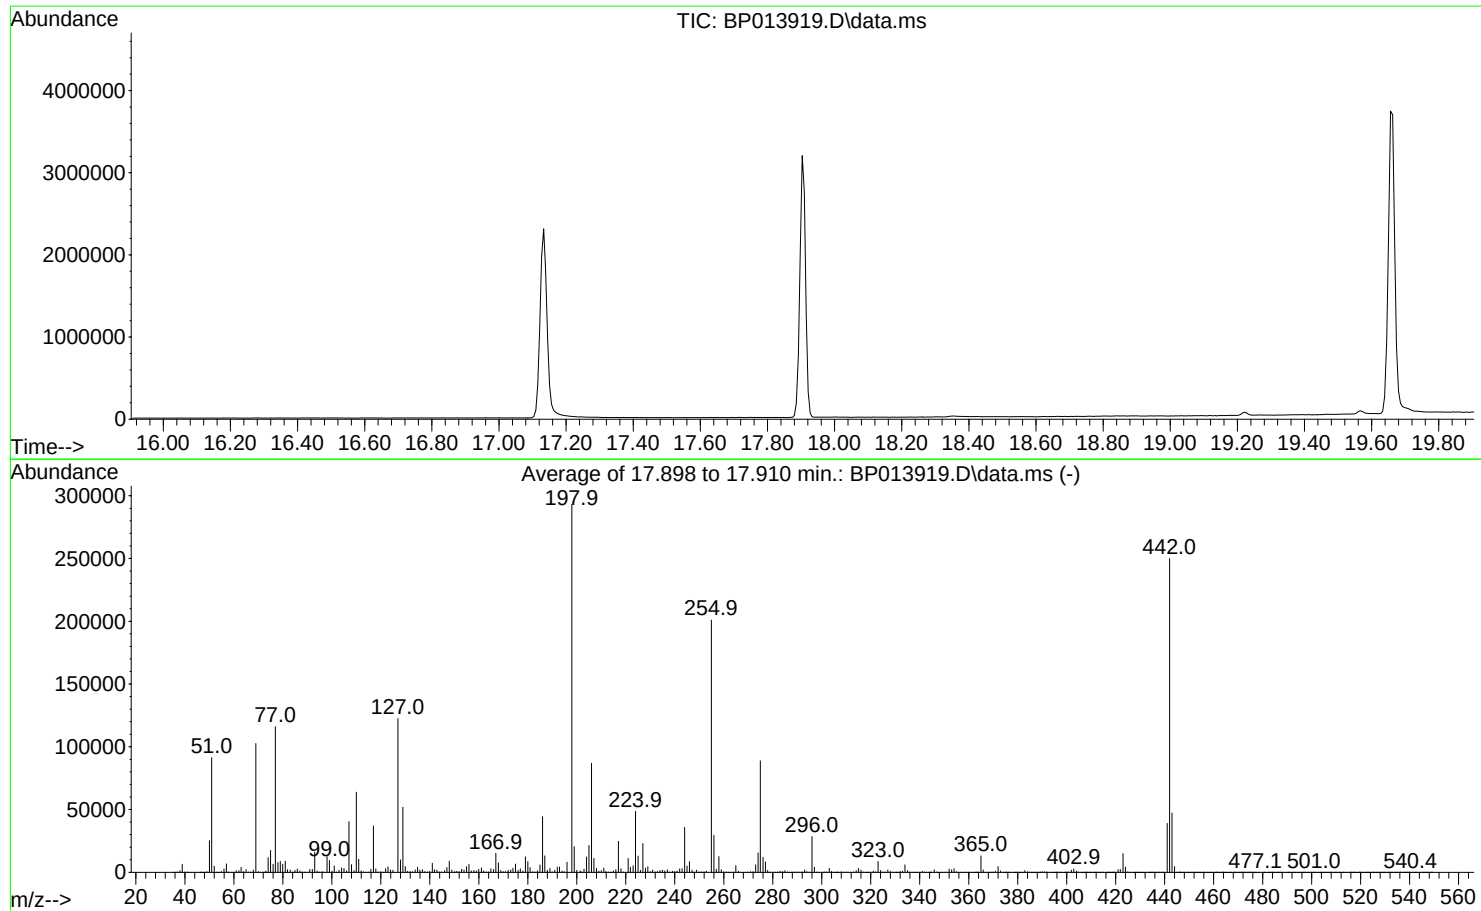




AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2492

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.2	91298	PASS
68	69	0.00	2	1.8	1837	PASS
69	198	0.00	100	35.0	102499	PASS
70	69	0.00	2	0.6	587	PASS
127	198	10	80	41.8	122430	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	293077	PASS
199	198	5	9	7.0	20430	PASS
275	198	10	60	30.3	88815	PASS
365	198	1	100	4.5	13133	PASS
441	198	0.01	100	13.3	39016	PASS
442	442	100	100	100.0	249920	PASS
443	442	15	24	18.9	47277	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030223\
Data File : BP013919.D
Acq On : 02 Mar 2023 13:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 03 05:51:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 02 04:26:35 2023
Response via : Initial Calibration

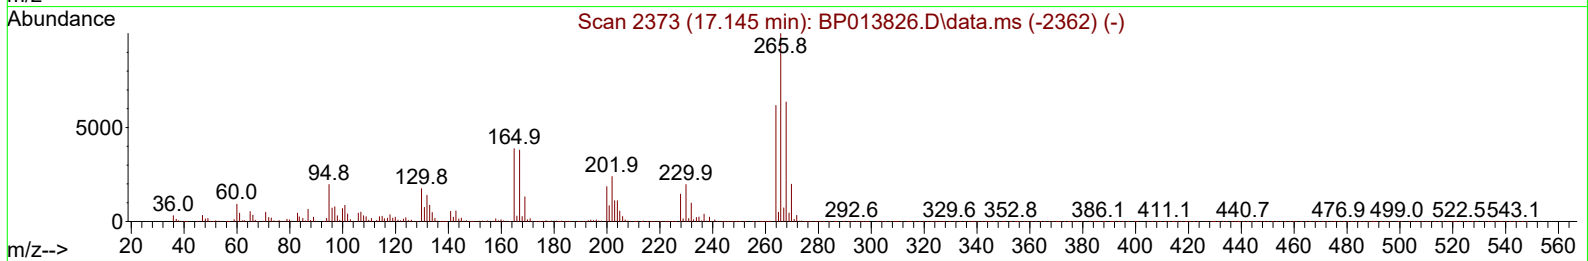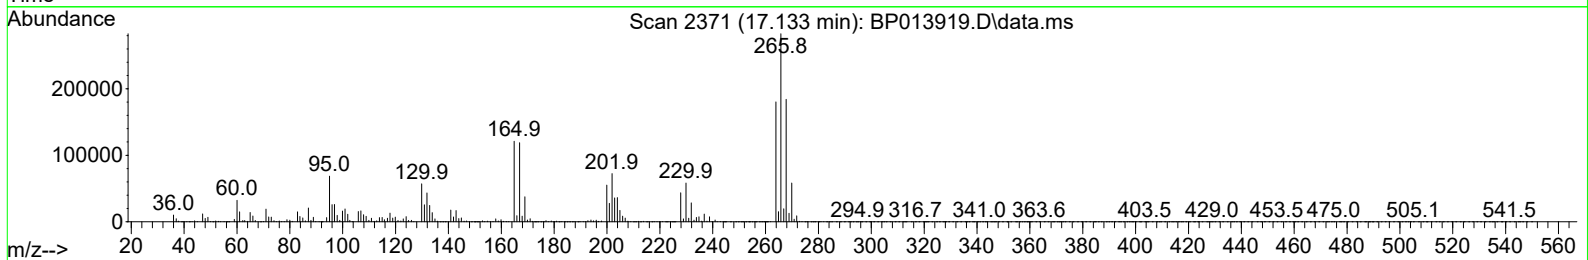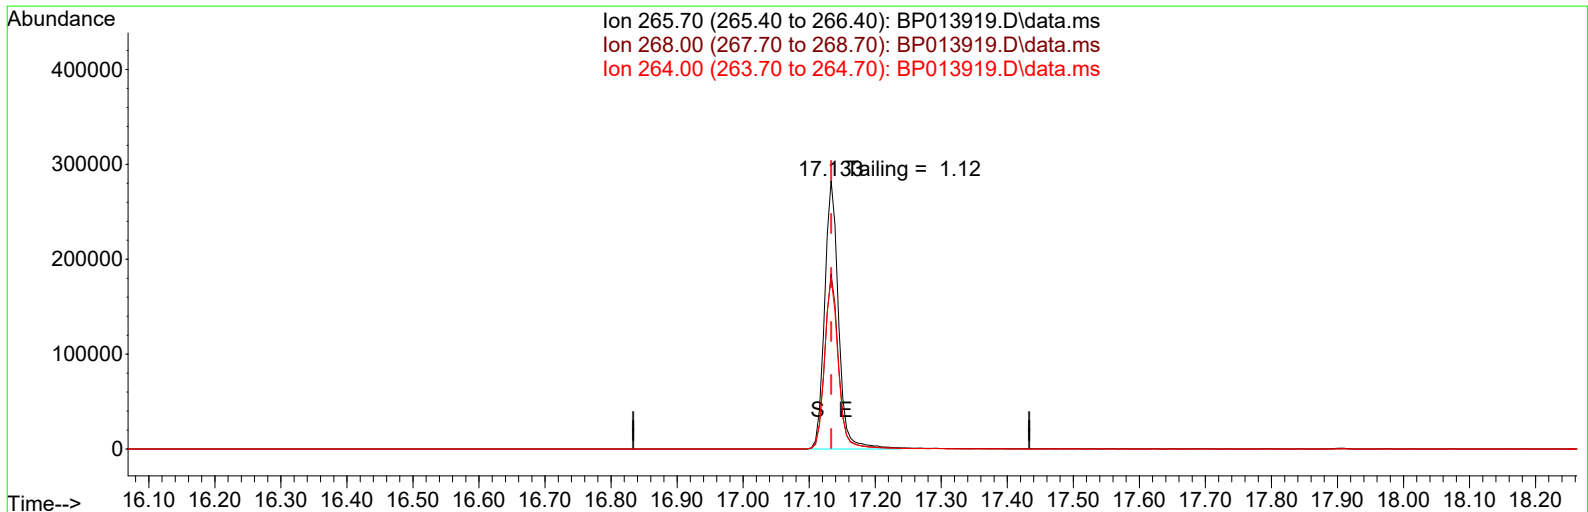

TIC: BP013919.D\data.ms

(70) Pentachlorophenol (C)

17.133min (-0.000) 1755427.03 ng




response 416876

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	65.13
264.00	61.70	63.75
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030223\
Data File : BP013919.D
Acq On : 02 Mar 2023 13:24
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 03 05:51:44 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 02 04:26:35 2023
Response via : Initial Calibration

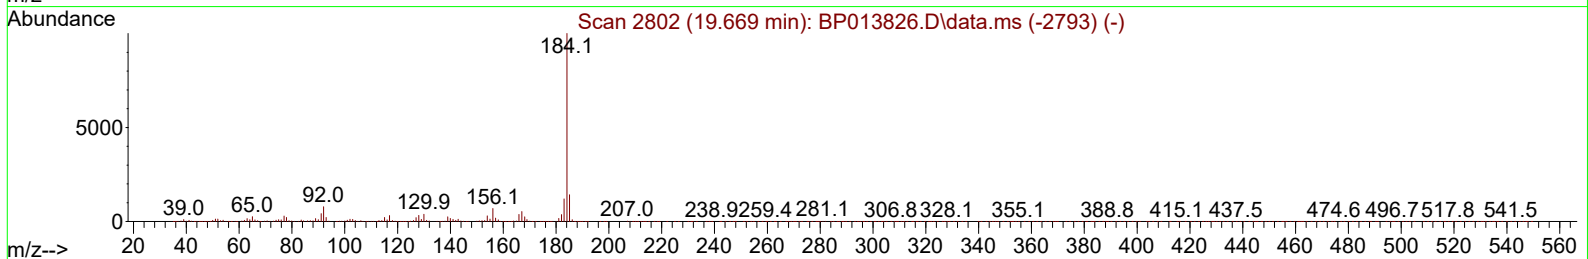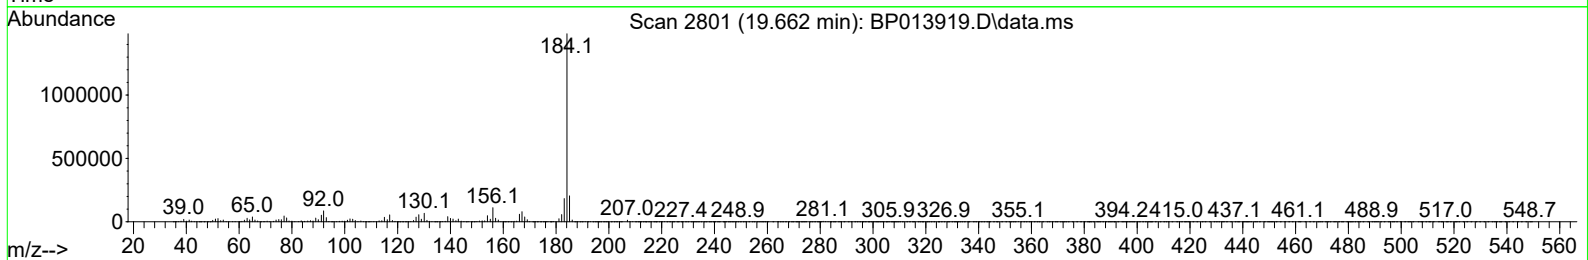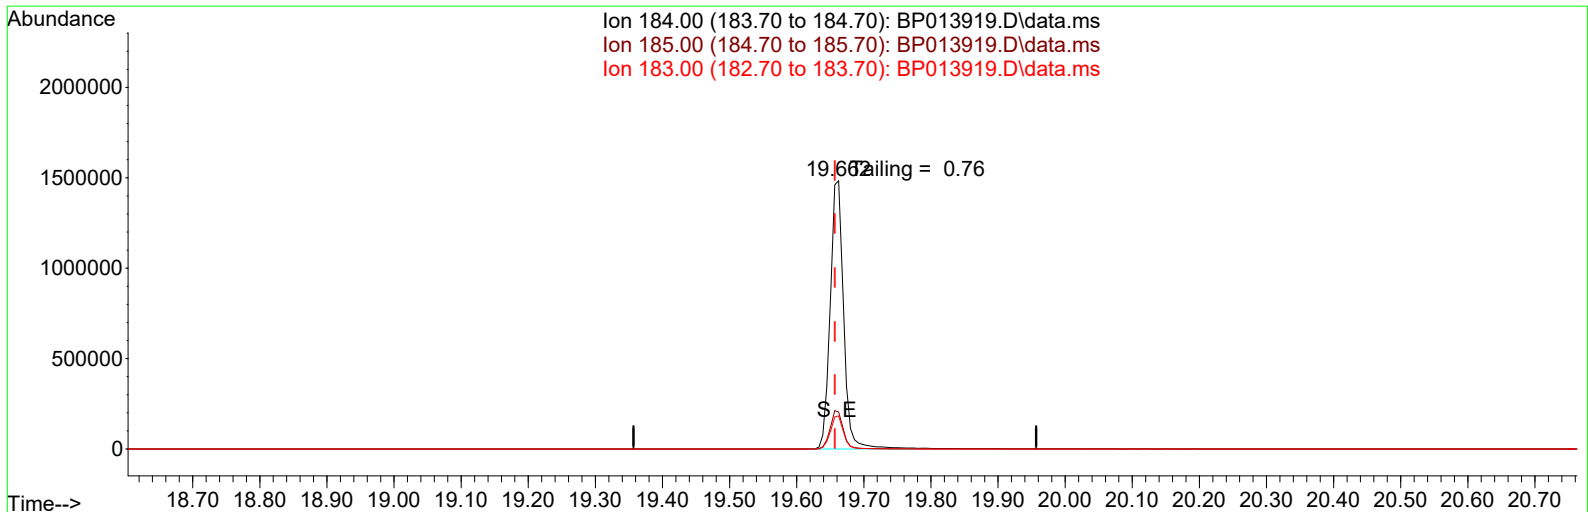

TIC: BP013919.D\data.ms

(77) Benzidine

19.662min (+ 0.006) 1437780.56 ng

response 2066939

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	13.76
183.00	12.00	12.37
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/2/2023	BNA_P	<u>BP013919.D</u>
Compound Name	Response	Retention Time
DDT	1021729	20.851
DDD	80580	20.421
DDE	1554	19.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
82134	1103863	7.44

Instrument :
BNA_P
ClientSampleId :
DFTPP