

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030322\
 Data File : BP009252.D
 Acq On : 03 Mar 2022 09:50
 Operator : CG/JU
 Sample : PB142783BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK783

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009252.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	11	14	23	rVB	72793	111834	1.37%	0.130%
2	3.323	53	57	68	rVB	99335	159758	1.96%	0.186%
3	3.723	121	125	142	rBV	1100065	1742510	21.36%	2.031%
4	4.052	178	181	187	rVB2	25065	38555	0.47%	0.045%
5	6.987	673	680	691	rBV	1423936	2335429	28.62%	2.722%
6	7.158	702	709	722	rBV	1083389	1886055	23.12%	2.199%
7	7.358	735	743	752	rBV	1408703	2396470	29.37%	2.794%
8	7.822	813	822	835	rBV	1152844	2000265	24.52%	2.332%
9	8.528	933	942	961	rBV	1661936	2885899	35.37%	3.364%
10	8.975	1010	1018	1031	rBV	1201899	2033318	24.92%	2.370%
11	9.699	1134	1141	1154	rBV	854254	1455144	17.84%	1.696%
12	10.234	1223	1232	1242	rBV	1638267	2883081	35.34%	3.361%
13	10.616	1289	1297	1309	rVB	1533528	2821783	34.59%	3.289%
14	10.752	1312	1320	1335	rBV	1631086	2975803	36.47%	3.469%
15	12.210	1561	1568	1576	rVB2	30612	55234	0.68%	0.064%
16	13.428	1771	1775	1777	rBV4	5787	9159	0.11%	0.011%
17	13.875	1844	1851	1865	rBV	2878540	4185977	51.31%	4.880%
18	14.151	1890	1898	1911	rBV	3397150	5247240	64.31%	6.117%
19	14.463	1944	1951	1960	rBV	2356016	3739496	45.83%	4.359%
20	14.645	1975	1982	1998	rBV	1092530	1666901	20.43%	1.943%
21	15.457	2113	2120	2132	rBV	4146073	6398056	78.42%	7.458%
22	15.569	2133	2139	2148	rBV	747866	1071441	13.13%	1.249%
23	15.698	2157	2161	2166	rVB2	20100	34269	0.42%	0.040%
24	16.140	2233	2236	2240	rVB5	5846	9662	0.12%	0.011%
25	16.257	2252	2256	2260	rVB7	6377	10441	0.13%	0.012%
26	16.904	2361	2366	2370	rBV7	7717	12445	0.15%	0.015%
27	17.004	2379	2383	2390	rVB	12987	23408	0.29%	0.027%
28	17.222	2413	2420	2430	rBV	2932883	4371623	53.58%	5.096%
29	17.322	2430	2437	2454	rVV2	4441334	6828915	83.70%	7.961%
30	19.145	2743	2747	2752	rVB3	59671	84717	1.04%	0.099%
31	19.210	2754	2758	2762	rVV	54709	75994	0.93%	0.089%
32	19.569	2812	2819	2831	rBV	5743854	8081170	99.05%	9.420%
33	21.327	3113	3118	3126	rVB	3823958	4852403	59.47%	5.657%
34	23.580	3494	3501	3513	rVB	3888947	8158853	100.00%	9.511%
35	23.739	3521	3528	3537	rVB2	2393146	5140688	63.01%	5.993%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030322\
Data File : BP009252.D
Acq On : 03 Mar 2022 09:50
Operator : CG/JU
Sample : PB142783BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK783

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Title : SVOA CALIBRATION




Sum of corrected areas: 85783996

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030322\
Data File : BP009252.D
Acq On : 03 Mar 2022 09:50
Operator : CG/JU
Sample : PB142783BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK783

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

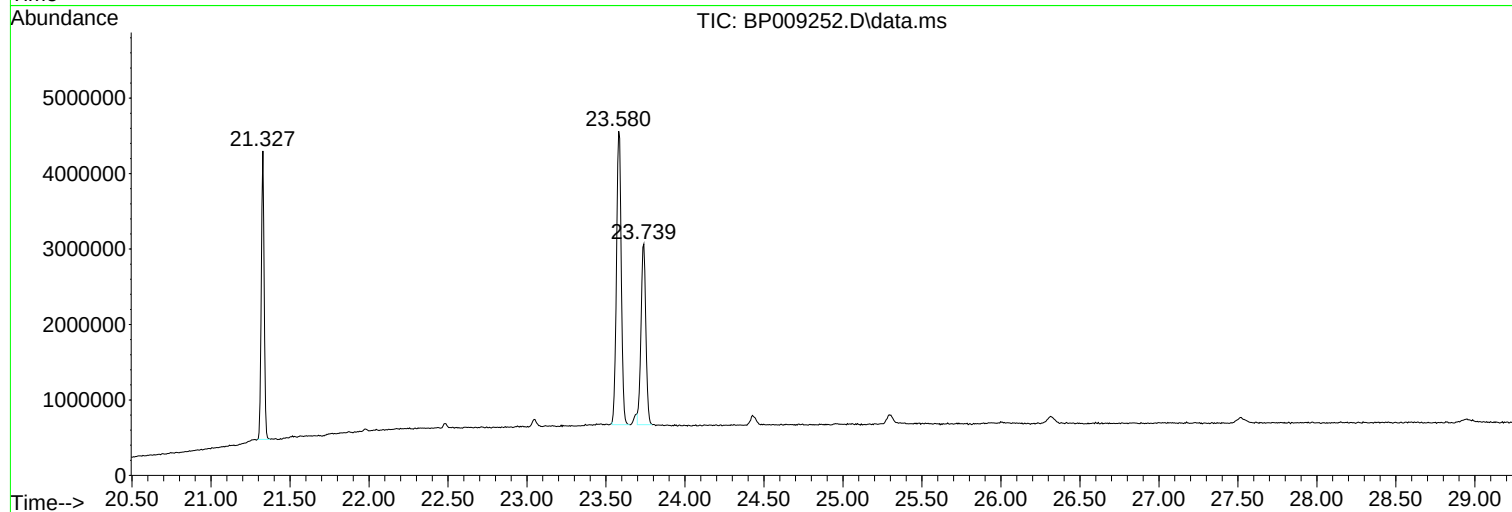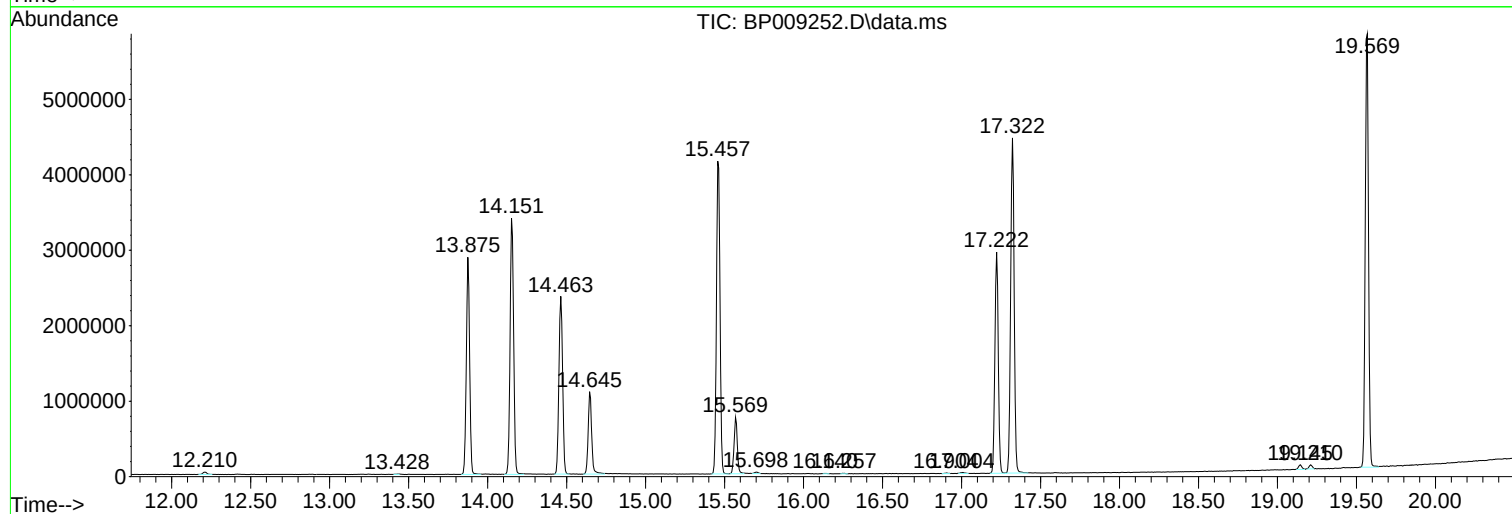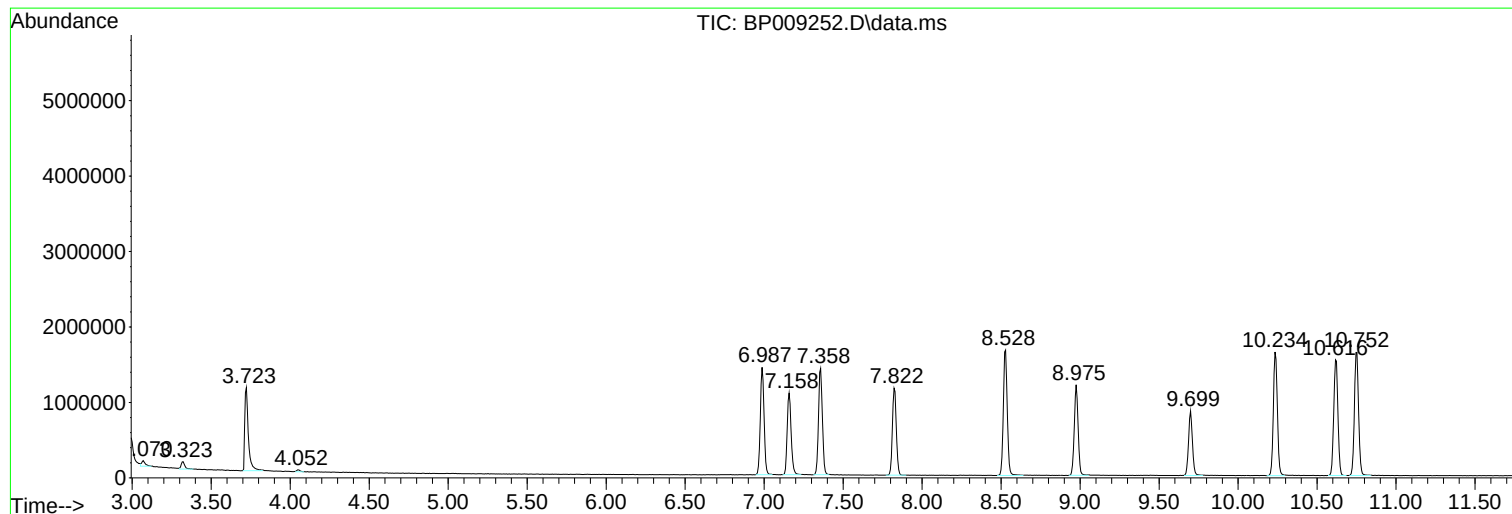

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030322\
Data File : BP009252.D
Acq On : 03 Mar 2022 09:50
Operator : CG/JU
Sample : PB142783BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK783

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030322\
Data File : BP009252.D
Acq On : 03 Mar 2022 09:50
Operator : CG/JU
Sample : PB142783BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK783

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc