

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030322\
 Data File : BP009254.D
 Acq On : 03 Mar 2022 11:10
 Operator : CG/JU
 Sample : PB142782BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK782

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009254.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	11	14	32	rVB2	87669	216133	2.81%	0.256%
2	3.322	53	57	69	rVB	105713	169162	2.20%	0.201%
3	3.722	122	125	143	rBV	1175863	1832474	23.80%	2.173%
4	4.052	178	181	189	rVB	29633	46175	0.60%	0.055%
5	5.034	344	348	349	rBV4	6518	9198	0.12%	0.011%
6	6.993	673	681	691	rBV	1438626	2400157	31.17%	2.846%
7	7.163	703	710	723	rBV	1099546	1917377	24.90%	2.274%
8	7.358	736	743	757	rVB	1421386	2459392	31.94%	2.916%
9	7.828	816	823	832	rBV	1200619	2039568	26.49%	2.418%
10	8.528	935	942	954	rBV	1707656	2923083	37.96%	3.466%
11	8.981	1011	1019	1033	rBV	1214584	2095145	27.21%	2.484%
12	9.704	1134	1142	1154	rBV	864653	1480681	19.23%	1.756%
13	10.240	1225	1233	1250	rBV	1666266	2910065	37.80%	3.451%
14	10.622	1290	1298	1309	rBV	1548930	2850264	37.02%	3.380%
15	10.757	1312	1321	1337	rBV	1666689	3000830	38.97%	3.558%
16	12.216	1562	1569	1575	rBV	32915	57313	0.74%	0.068%
17	12.434	1597	1606	1608	rBV9	4524	8021	0.10%	0.010%
18	13.198	1731	1736	1741	rBV8	5047	11543	0.15%	0.014%
19	13.440	1768	1777	1785	rBV7	6974	15213	0.20%	0.018%
20	13.881	1844	1852	1865	rBV	2792049	4102641	53.28%	4.865%
21	14.157	1891	1899	1910	rBV	3337060	5184763	67.34%	6.148%
22	14.469	1945	1952	1960	rBV	2419762	3715384	48.25%	4.405%
23	14.651	1976	1983	2005	rBV	1030856	1639973	21.30%	1.945%
24	15.469	2114	2122	2133	rBV	4138249	6273542	81.48%	7.439%
25	15.575	2134	2140	2150	rBV	690823	1033521	13.42%	1.225%
26	15.704	2157	2162	2172	rVB2	21968	45400	0.59%	0.054%
27	16.145	2230	2237	2240	rBV8	9269	19643	0.26%	0.023%
28	16.263	2251	2257	2260	rVB8	5841	8936	0.12%	0.011%
29	17.010	2380	2384	2390	rVB2	13518	17930	0.23%	0.021%
30	17.228	2414	2421	2431	rBV	2908507	4205622	54.62%	4.987%
31	17.328	2431	2438	2449	rBV2	4304368	6575422	85.40%	7.797%
32	19.151	2744	2748	2752	rBV3	58523	79217	1.03%	0.094%
33	19.216	2755	2759	2763	rBV2	54131	76272	0.99%	0.090%
34	19.575	2813	2820	2831	rBV	5260023	7687644	99.84%	9.116%
35	21.333	3114	3119	3129	rBV	3515431	4592038	59.64%	5.445%
36	23.592	3496	3503	3515	rVB2	3717985	7699586	100.00%	9.130%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030322\
Data File : BP009254.D
Acq On : 03 Mar 2022 11:10
Operator : CG/JU
Sample : PB142782BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK782

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Title : SVOA CALIBRATION

37	23.745	3523	3529	3542	rVB2	2203812	4936578	64.11%	5.853%
----	--------	------	------	------	------	---------	---------	--------	--------




Sum of corrected areas: 84335906

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030322\
Data File : BP009254.D
Acq On : 03 Mar 2022 11:10
Operator : CG/JU
Sample : PB142782BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK782

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

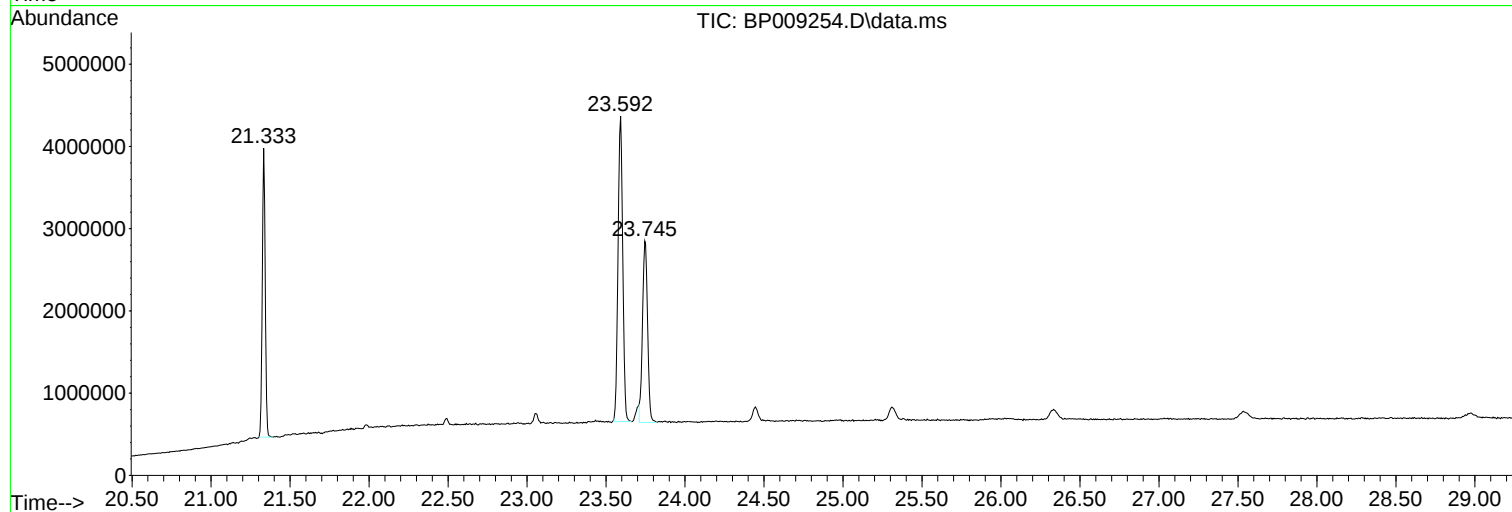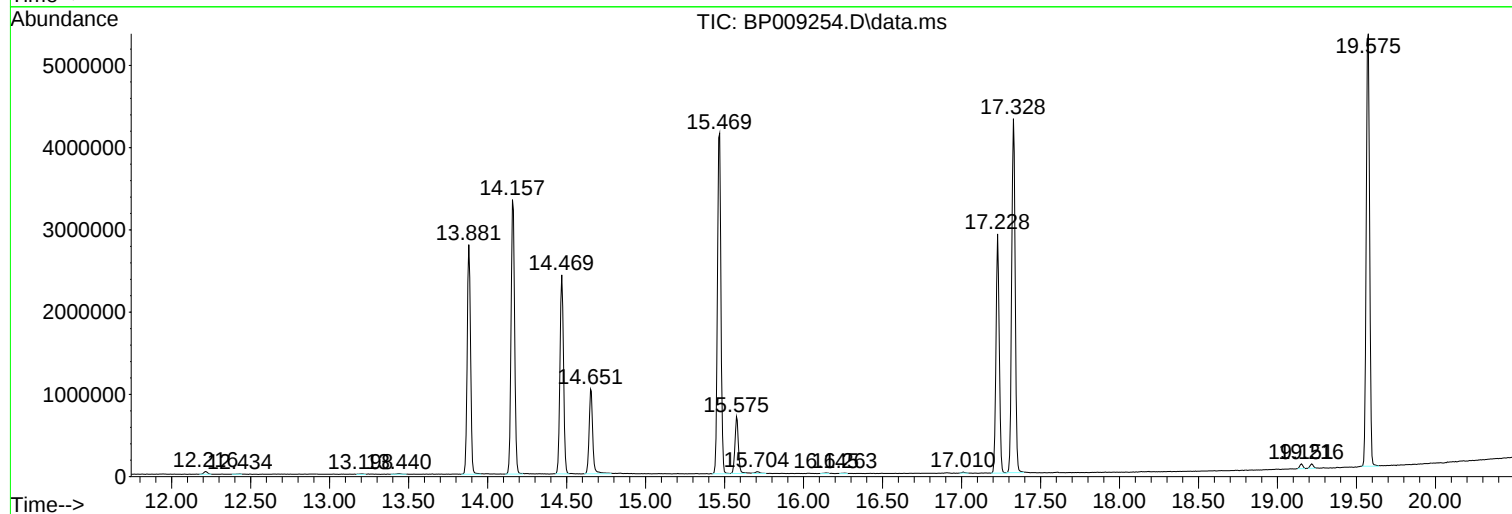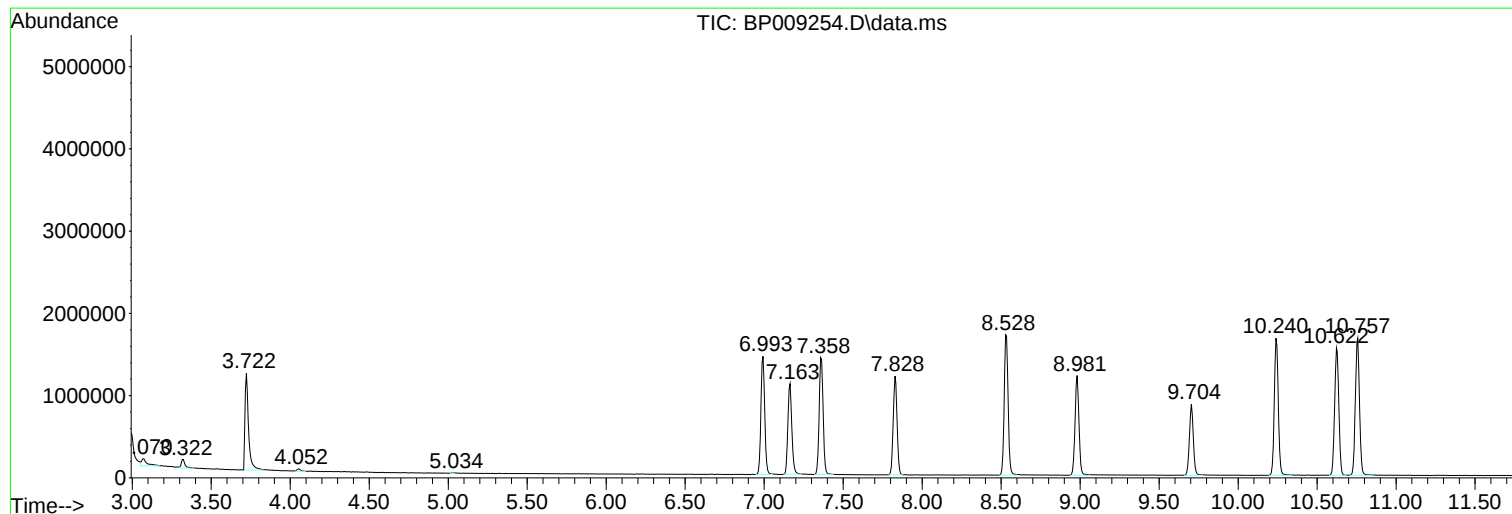

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030322\
Data File : BP009254.D
Acq On : 03 Mar 2022 11:10
Operator : CG/JU
Sample : PB142782BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK782










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown-01 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.070	2.12 ng/ul	216133	1,4-Dichlorobenzene-d4	7.828

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	45
2			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	38
3			1,3-Dioxolane, 2-pentadecyl-	284	C18H36O2	004360-57-0	14
4			1,3-Dioxolane, 2-(6-heptynyl)-	168	C10H16O2	025595-82-8	9
5			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9

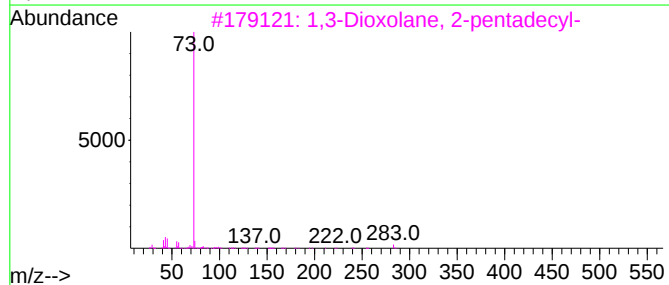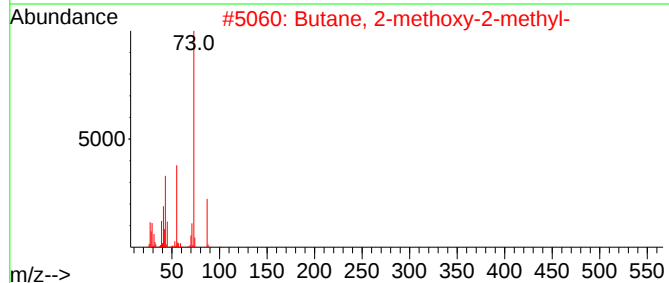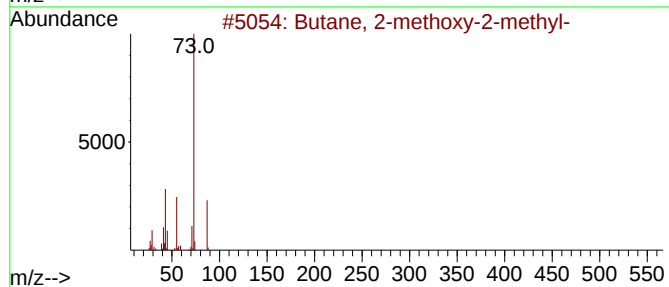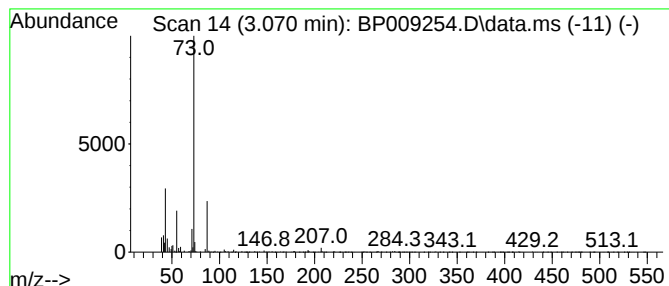

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030322\
Data File : BP009254.D
Acq On : 03 Mar 2022 11:10
Operator : CG/JU
Sample : PB142782BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK782

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown-01	3.070	2.1	ng/ul	216133	1	7.828	2039570	20.0