

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030322\
 Data File : BP009256.D
 Acq On : 03 Mar 2022 12:29
 Operator : CG/JU
 Sample : PB142786BL
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK786

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
 Title : SVOA CALIBRATION

Signal : TIC: BP009256.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.070	11	14	22	rVB	70988	106257	1.42%	0.126%
2	3.317	53	56	71	rVB	113695	190209	2.54%	0.226%
3	3.723	121	125	145	rBV	1191392	1883988	25.19%	2.235%
4	4.052	177	181	186	rBV	26784	39038	0.52%	0.046%
5	6.993	673	681	691	rBV	1480987	2487037	33.25%	2.950%
6	7.164	702	710	725	rBV	1130083	1998040	26.72%	2.370%
7	7.358	736	743	757	rVB	1483556	2533453	33.87%	3.005%
8	7.828	815	823	832	rBV	1239184	2081185	27.83%	2.469%
9	8.528	934	942	959	rBV	1768226	3021129	40.39%	3.584%
10	8.981	1009	1019	1033	rBV	1266527	2161656	28.90%	2.564%
11	9.705	1133	1142	1154	rBV	873493	1532334	20.49%	1.818%
12	10.240	1225	1233	1249	rBV	1690647	2990888	39.99%	3.548%
13	10.622	1289	1298	1308	rBV	1625833	2932346	39.21%	3.478%
14	10.752	1312	1320	1337	rBV	1729232	3083517	41.23%	3.658%
15	12.216	1563	1569	1574	rBV2	34831	59570	0.80%	0.071%
16	13.204	1730	1737	1741	rBV10	4012	8051	0.11%	0.010%
17	13.440	1770	1777	1781	rBV6	8100	19019	0.25%	0.023%
18	13.881	1845	1852	1866	rBV	2833503	4173384	55.80%	4.950%
19	14.157	1890	1899	1908	rBV	3286650	5249933	70.20%	6.227%
20	14.469	1944	1952	1960	rBV	2485057	3801047	50.82%	4.509%
21	14.651	1973	1983	2001	rBV	1105250	1656002	22.14%	1.964%
22	14.828	2010	2013	2018	rVV7	4391	7928	0.11%	0.009%
23	15.463	2114	2121	2131	rBV	4201621	6345768	84.85%	7.527%
24	15.575	2134	2140	2152	rBV	745152	1075681	14.38%	1.276%
25	15.704	2158	2162	2171	rVB2	21665	40619	0.54%	0.048%
26	16.251	2251	2255	2260	rBV8	6327	9800	0.13%	0.012%
27	16.910	2362	2367	2371	rVB7	5972	12010	0.16%	0.014%
28	17.010	2380	2384	2390	rVB	10842	16260	0.22%	0.019%
29	17.228	2414	2421	2430	rBV	2860381	4204329	56.22%	4.987%
30	17.328	2431	2438	2448	rBV	4393751	6513085	87.09%	7.725%
31	19.151	2743	2748	2753	rBV2	56078	81300	1.09%	0.096%
32	19.216	2755	2759	2764	rVV	52853	75009	1.00%	0.089%
33	19.569	2813	2819	2832	rBV	5305672	7478973	100.00%	8.871%
34	21.333	3114	3119	3125	rBV	3354729	4375081	58.50%	5.190%
35	23.586	3495	3502	3513	rVB2	3441943	7405139	99.01%	8.784%
36	23.745	3523	3529	3541	rVB2	2204340	4657322	62.27%	5.524%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030322\
Data File : BP009256.D
Acq On : 03 Mar 2022 12:29
Operator : CG/JU
Sample : PB142786BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK786

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Title : SVOA CALIBRATION




Sum of corrected areas: 84306387

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030322\
Data File : BP009256.D
Acq On : 03 Mar 2022 12:29
Operator : CG/JU
Sample : PB142786BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK786

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

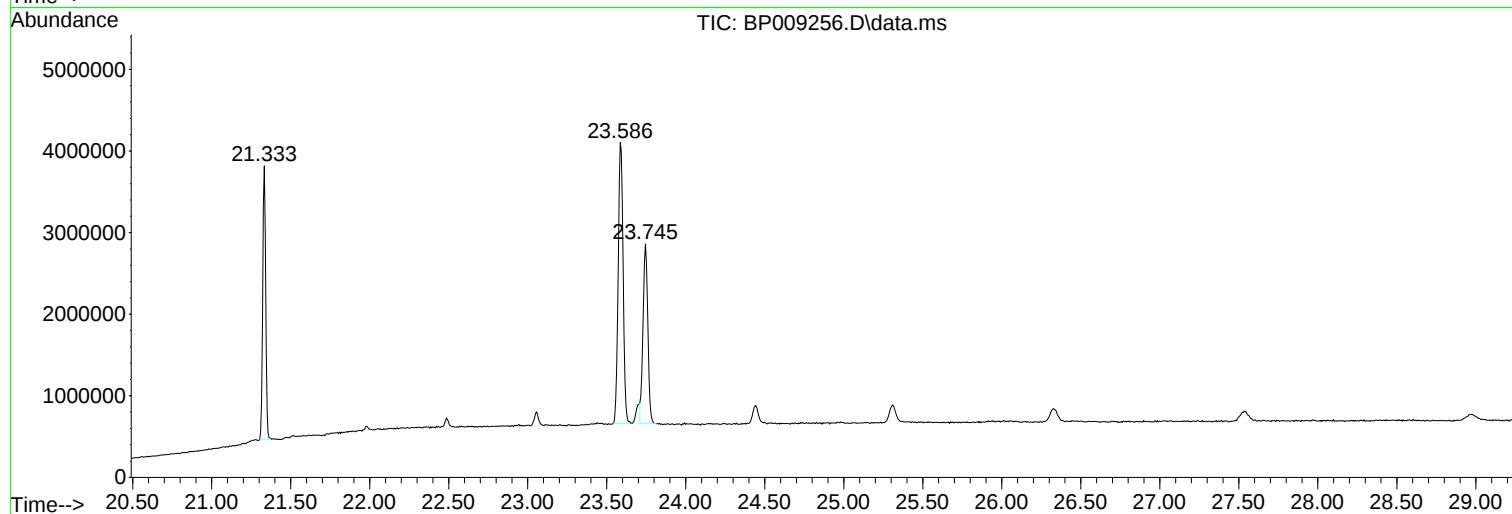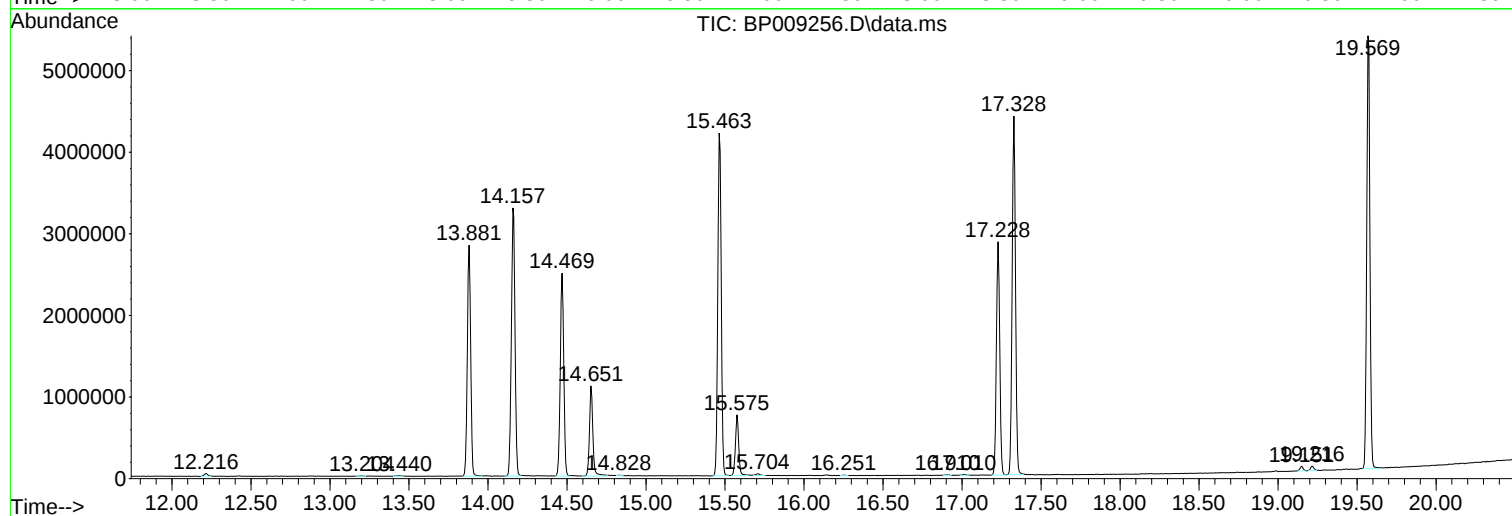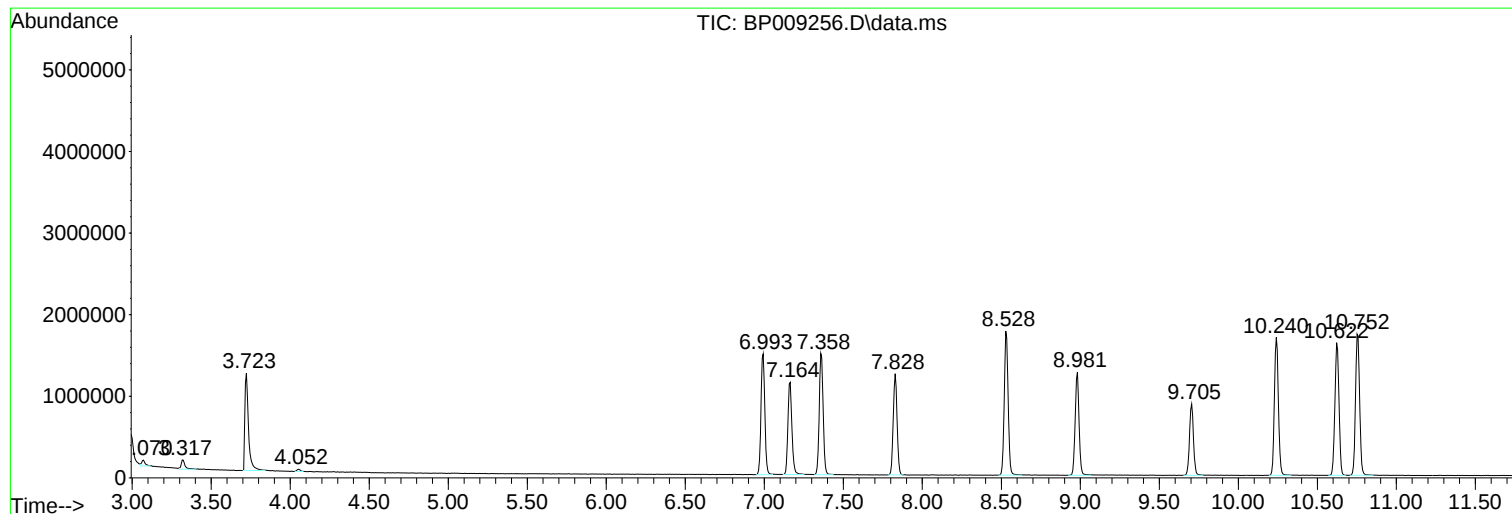

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030322\
Data File : BP009256.D
Acq On : 03 Mar 2022 12:29
Operator : CG/JU
Sample : PB142786BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK786

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030322\
Data File : BP009256.D
Acq On : 03 Mar 2022 12:29
Operator : CG/JU
Sample : PB142786BL
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK786

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030222.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc