
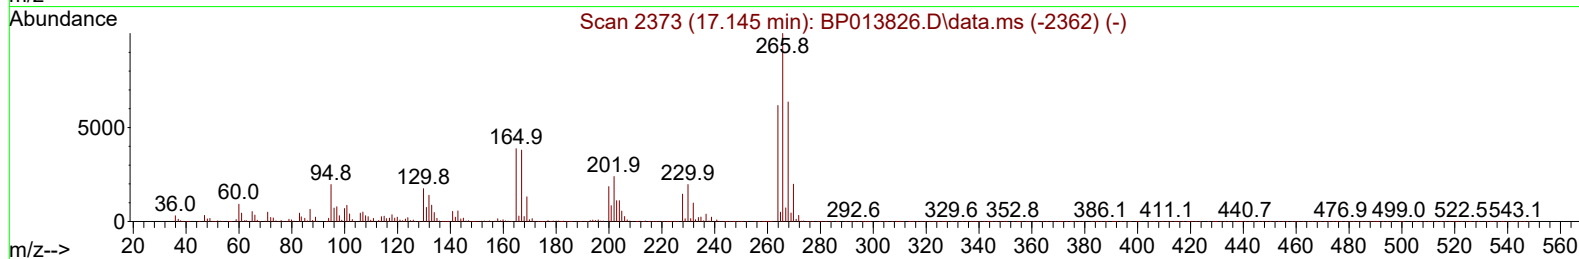
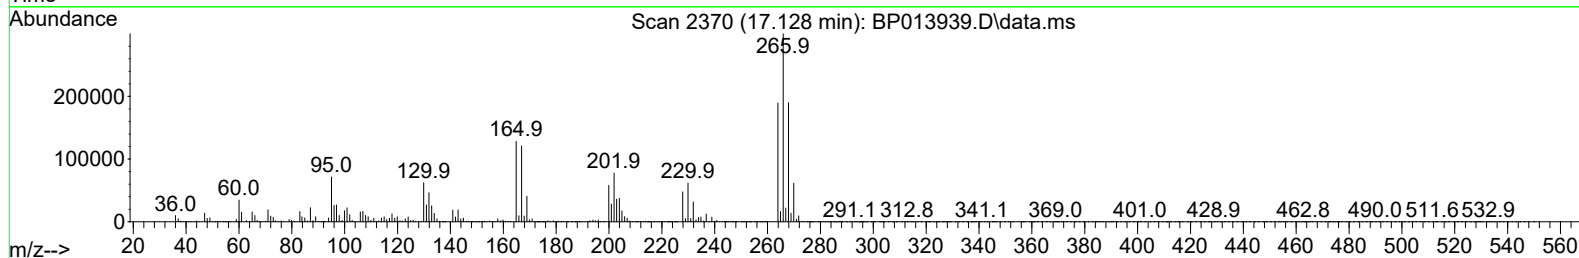


Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP030323\  
Data File : BP013939.D  
Acq On : 03 Mar 2023 11:53  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 04 02:31:42 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP021623.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 02 04:26:35 2023  
Response via : Initial Calibration

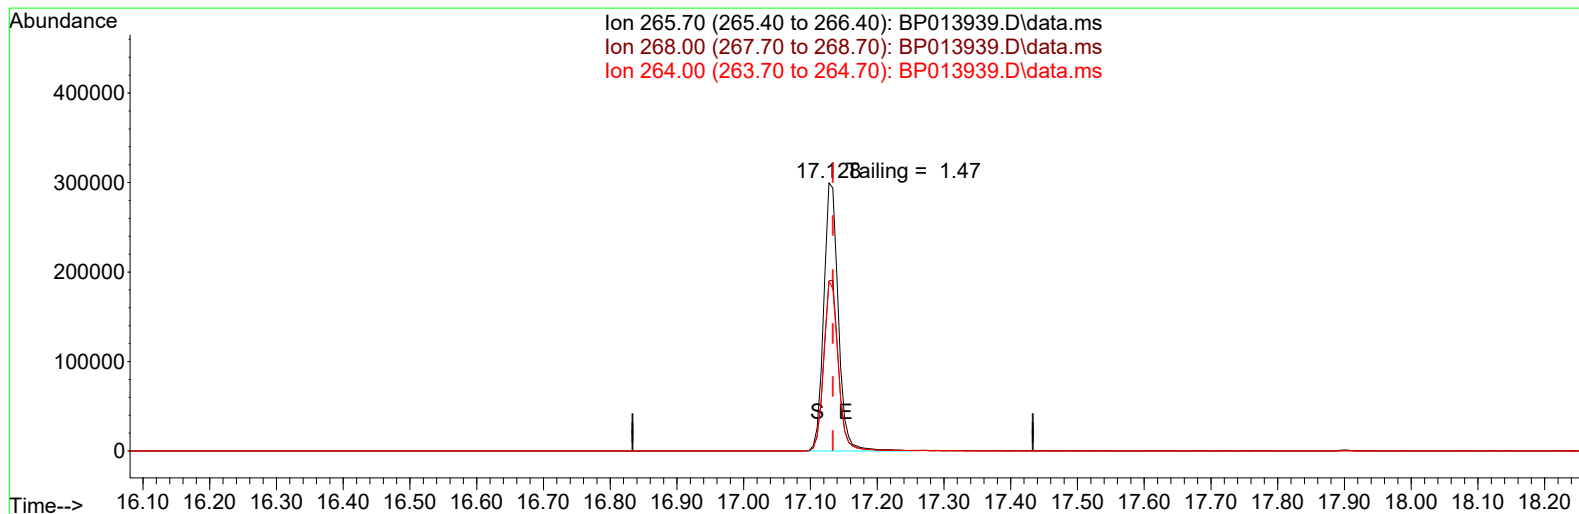

TIC: BP013939.D\data.ms

**(70) Pentachlorophenol (C)**




**17.128min (-0.006) 3434297.33 ng**

**response 456720**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.60  | 63.40  |
| 264.00 | 61.70  | 63.19  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_P\Data\BP030323\  
Data File : BP013939.D  
Acq On : 03 Mar 2023 11:53  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 04 02:31:42 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_P\Methods\8270E-BP021623.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Mar 02 04:26:35 2023  
Response via : Initial Calibration

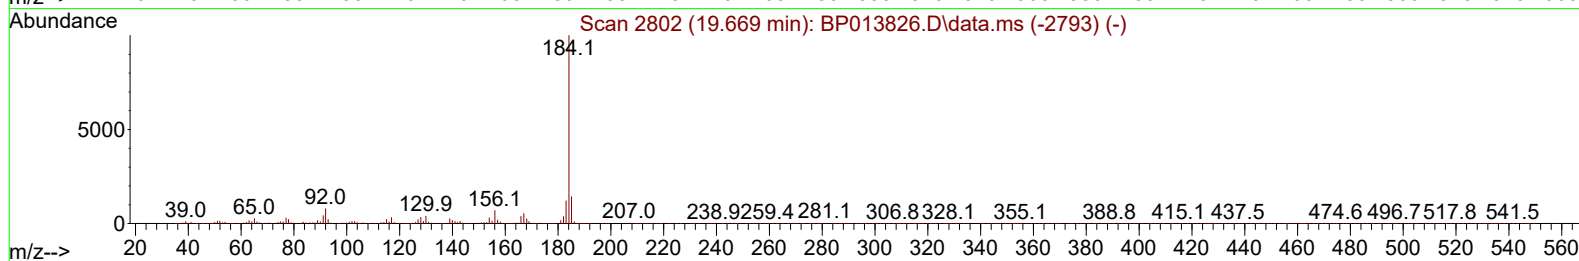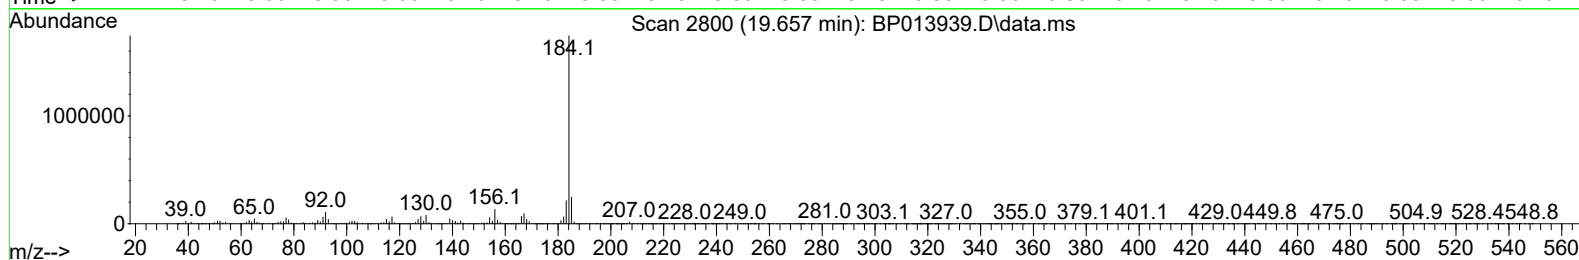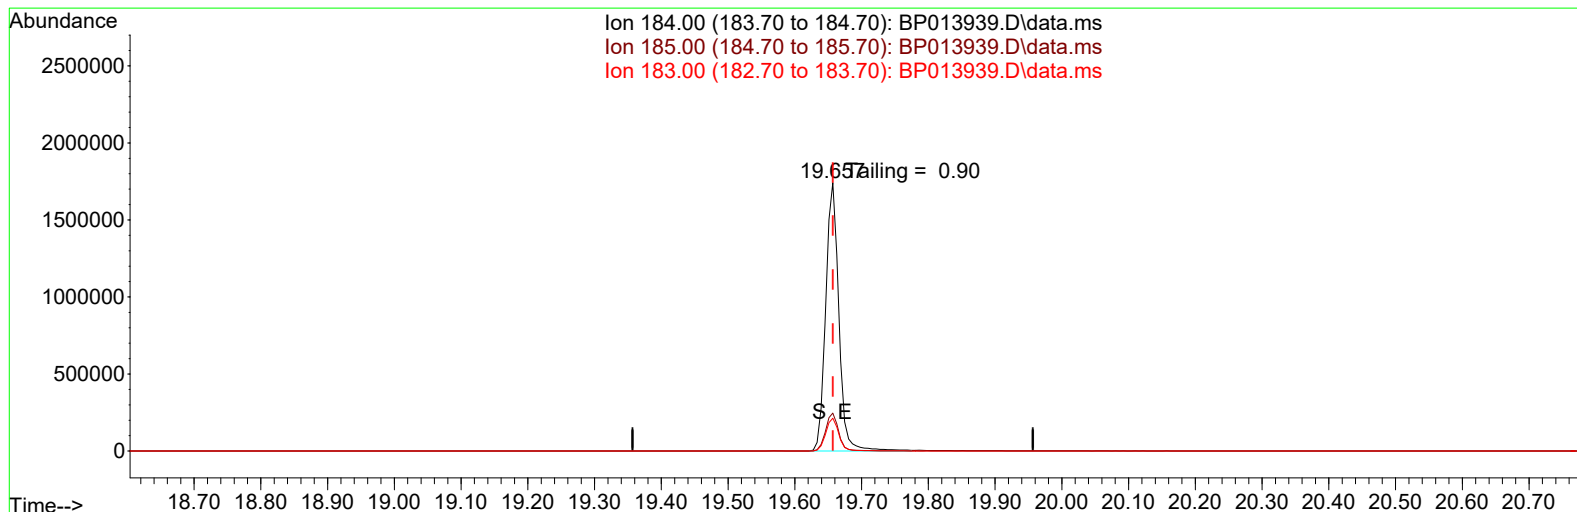

TIC: BP013939.D\data.ms

**(77) Benzidine****19.657min ( 0.000) 1310849.63 ng****response 2390738**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.20  | 14.12  |
| 183.00 | 12.00  | 12.25  |
| 0.00   | 0.00   | 0.00   |