
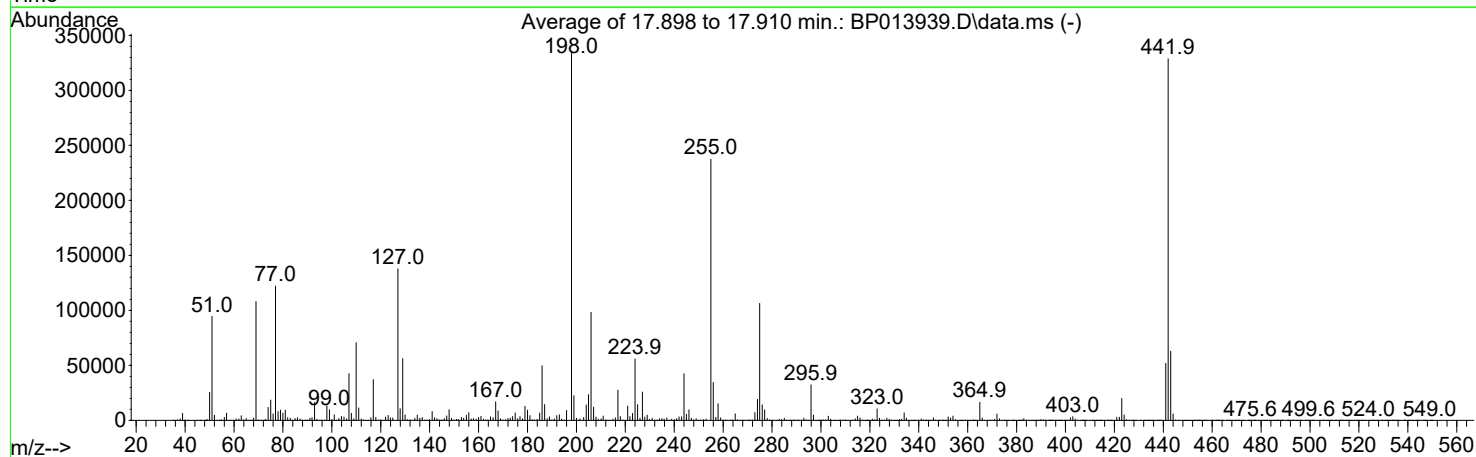


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030323\
 Data File : BP013939.D
 Acq On : 03 Mar 2023 11:53
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 02 04:26:35 2023

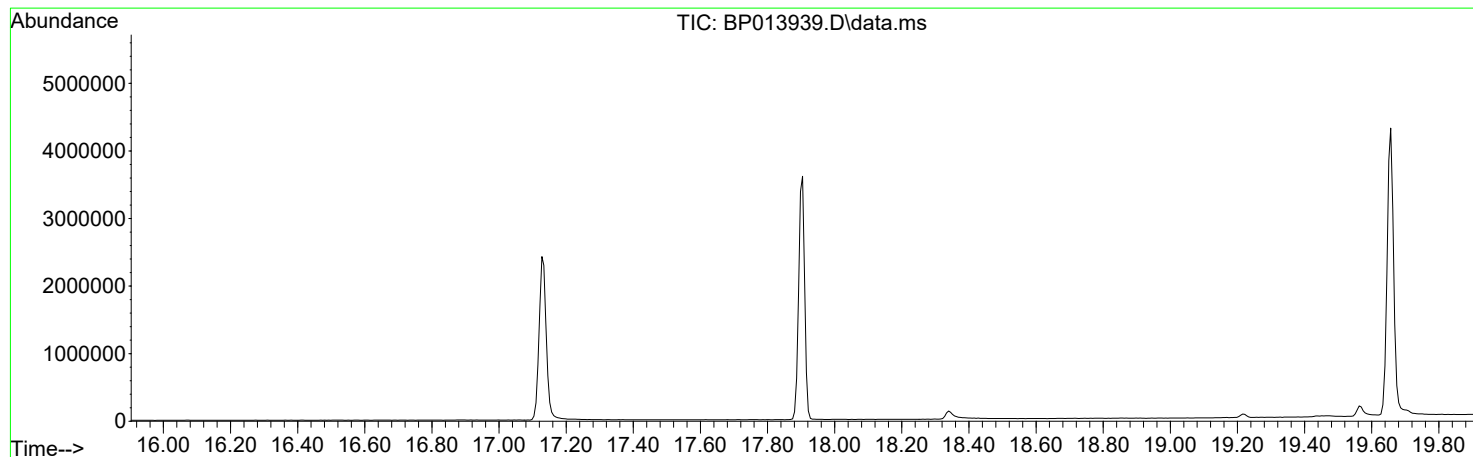

AutoFind: Scans 2501, 2502, 2503; Background Corrected with Scan 2488

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	28.3	94504	PASS
68	69	0.00	2	2.0	2117	PASS
69	198	0.00	100	32.3	108055	PASS
70	69	0.00	2	0.5	521	PASS
127	198	10	80	41.2	137763	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	334456	PASS
199	198	5	9	6.8	22628	PASS
275	198	10	60	31.8	106278	PASS
365	198	1	100	4.9	16410	PASS
441	198	0.01	100	15.5	51816	PASS
442	442	100	100	100.0	328719	PASS
443	442	15	24	19.1	62867	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/3/2023	BNA_P	<u>BP013939.D</u>
Compound Name	Response	Retention Time
DDT	1318586	20.851
DDD	17053	20.469
DDE	902	19.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
17955	1336541	1.34

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030323\
Data File : BP013939.D
Acq On : 03 Mar 2023 11:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 04 02:31:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 02 04:26:35 2023
Response via : Initial Calibration

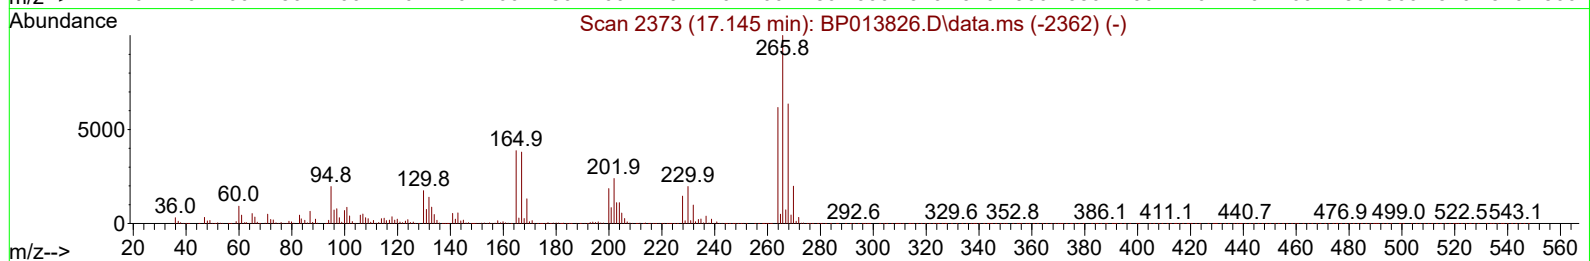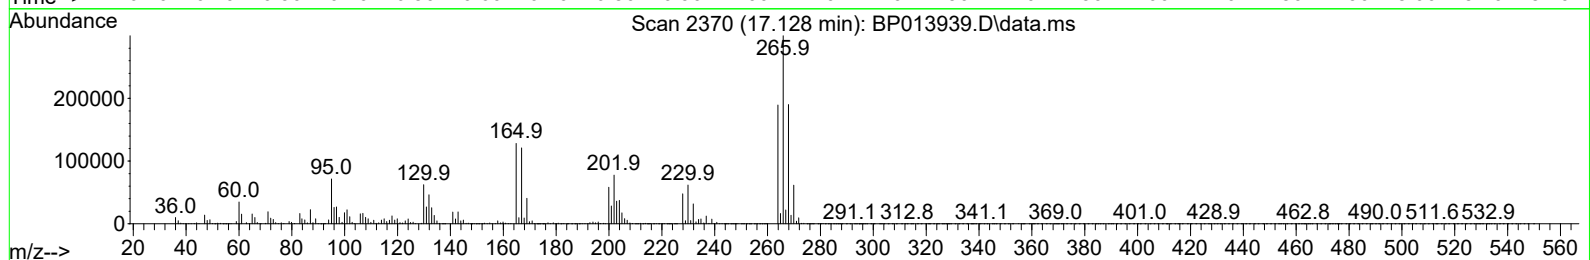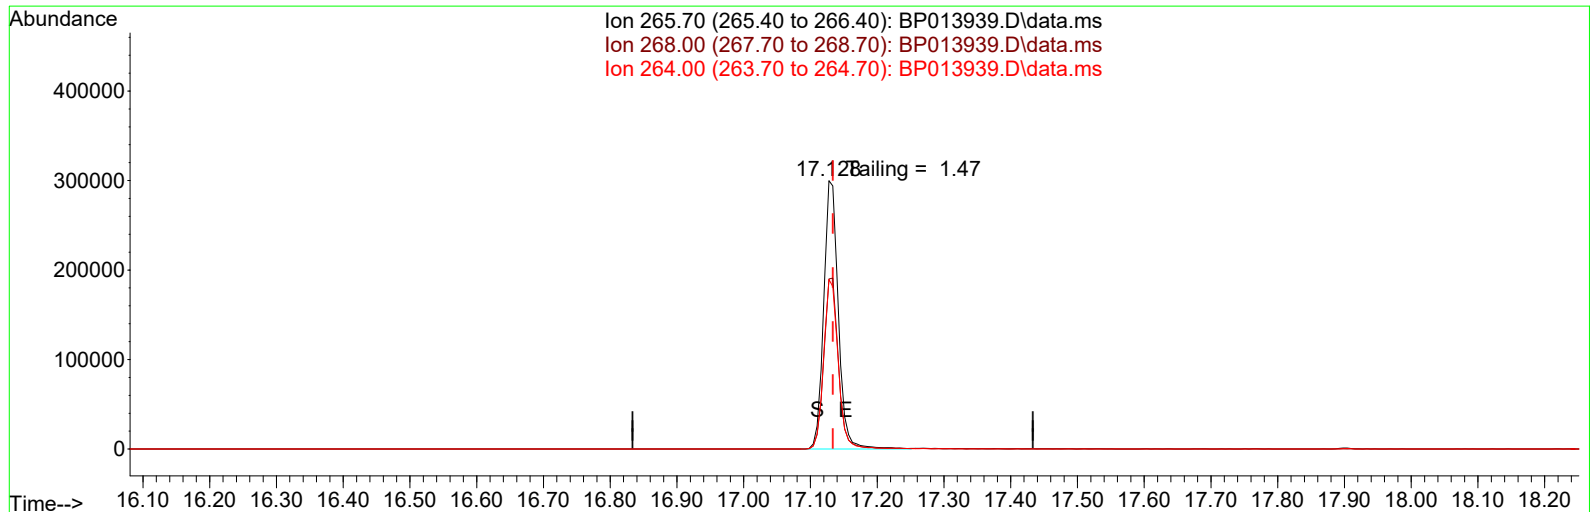

TIC: BP013939.D\data.ms

(70) Pentachlorophenol (C)

17.128min (-0.006) 3434297.33 ng




response 456720

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	63.40
264.00	61.70	63.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP030323\
Data File : BP013939.D
Acq On : 03 Mar 2023 11:53
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 04 02:31:42 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP021623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 02 04:26:35 2023
Response via : Initial Calibration

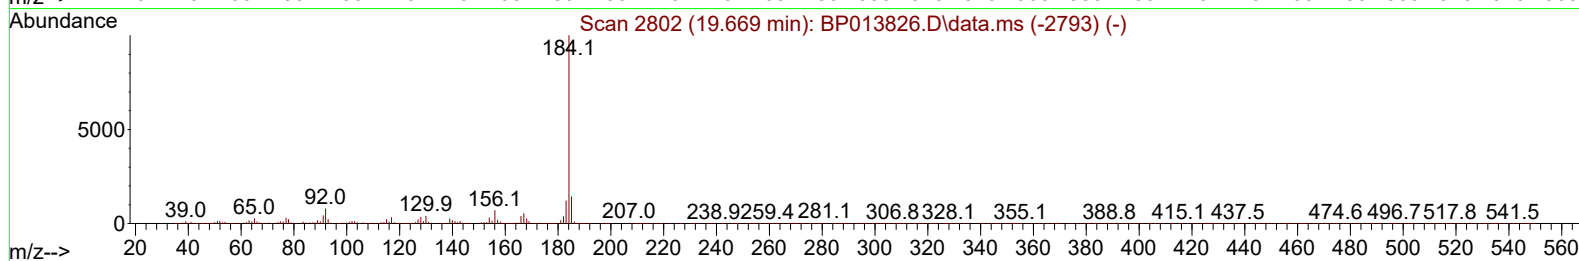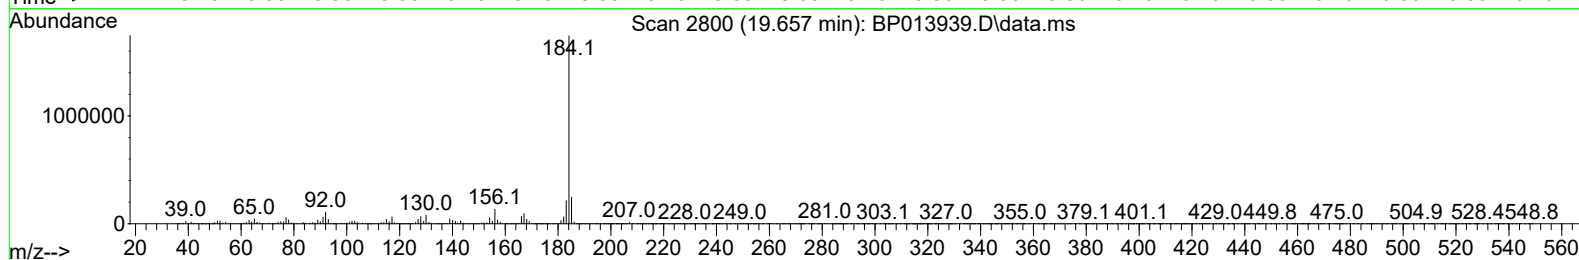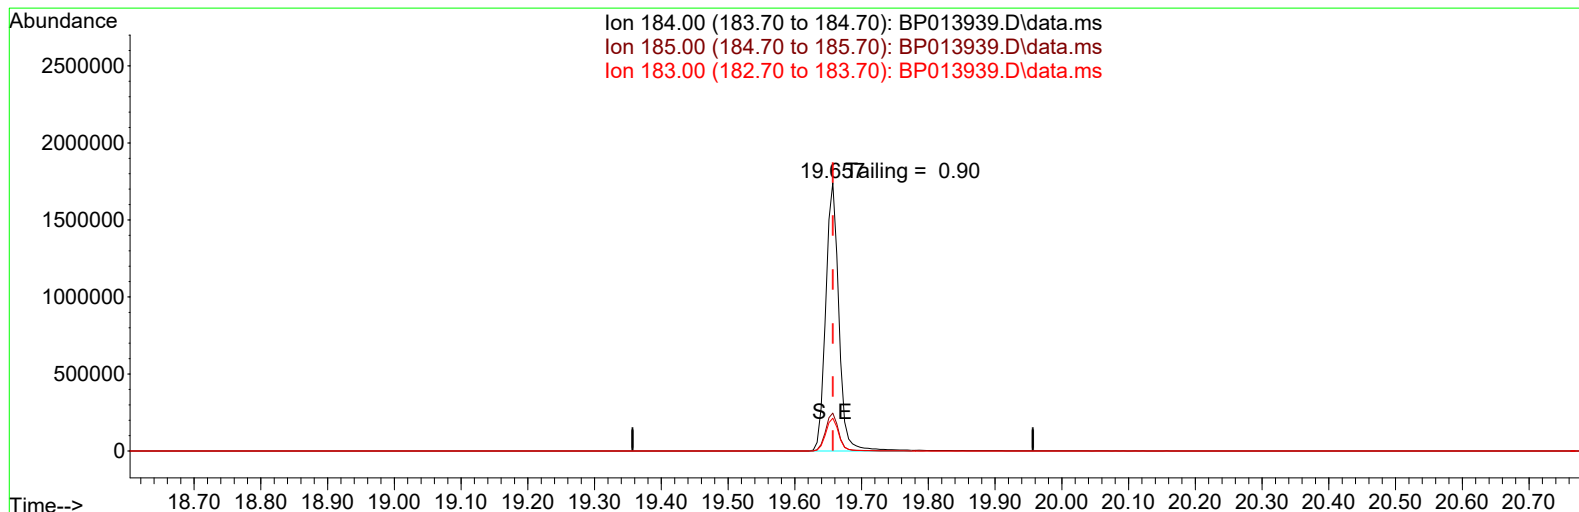

TIC: BP013939.D\data.ms

(77) Benzidine

19.657min (0.000) 1310849.63 ng

response 2390738

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.20	14.12
183.00	12.00	12.25
0.00	0.00	0.00