
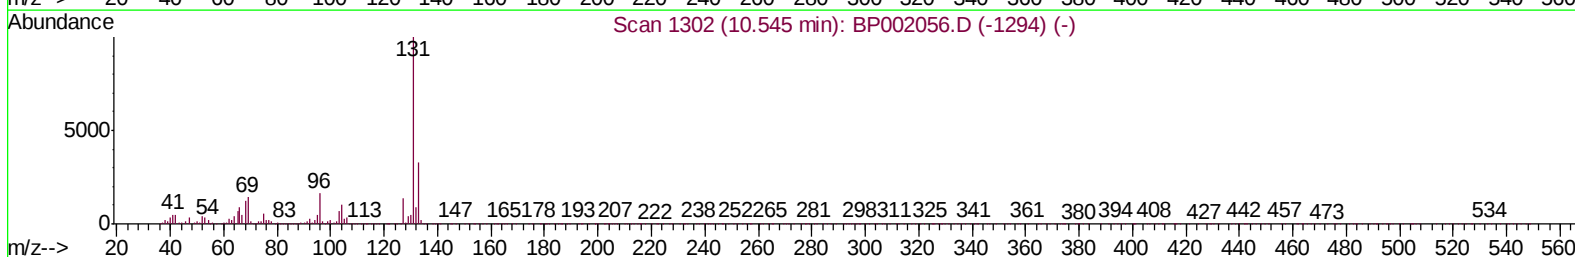
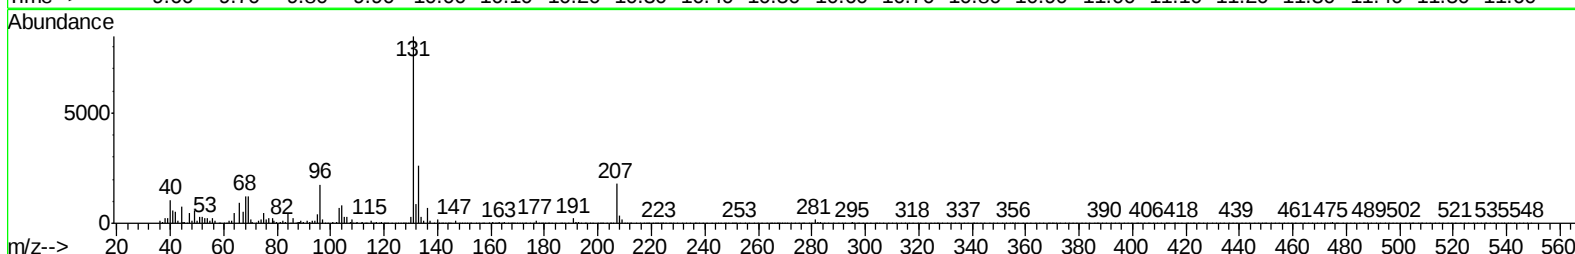


Data File : BP002063.D
Acq On : 04 Mar 2020 22:32
Operator : CG/JU
Sample : L1677-20
Misc :
ALS Vial : 22 Sample Multiplier: 1

Quant Time: Mar 05 06:24:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 05 06:21:29 2020
Response via : Initial Calibration

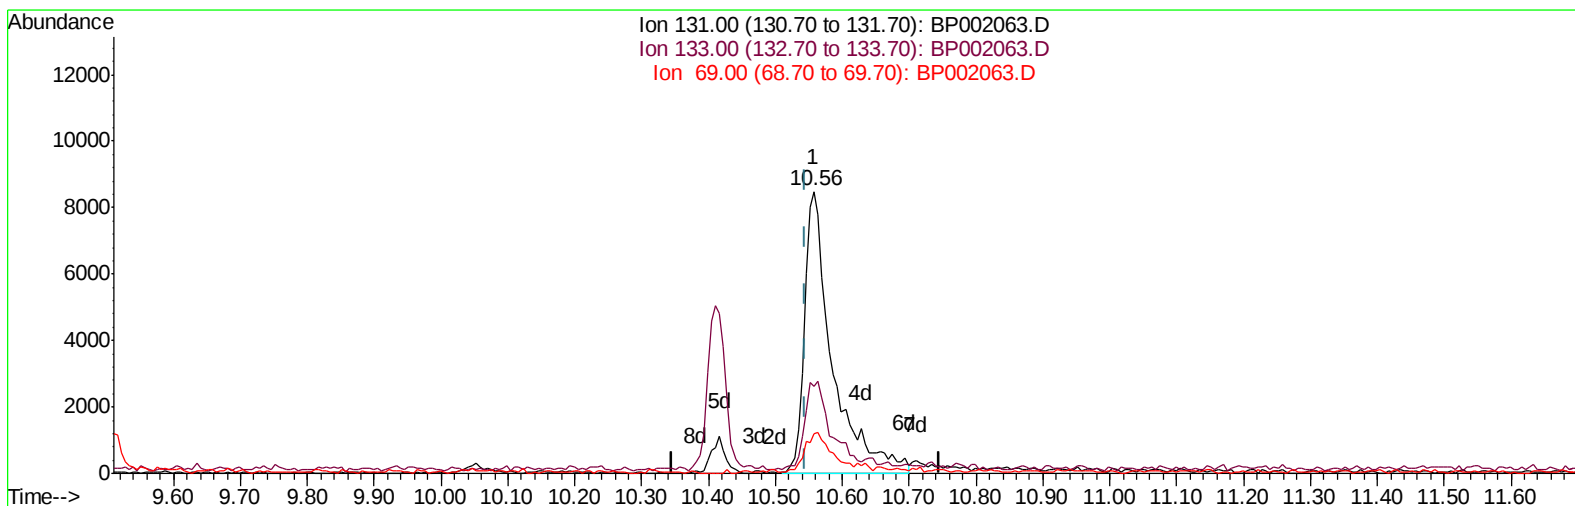

TIC: BP002063.D

(29) 4-Chloroaniline-d4 (S)

10.557min (+0.012) 1.12ng/ul m

response 24886

Ion	Exp%	Act%
131.00	100	100
133.00	32.40	30.74
69.00	15.50	14.13
0.00	0.00	0.00