

Data File : BP002060.D
Acq On : 04 Mar 2020 20:50
Operator : CG/JU
Sample : L1677-19
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CB6

Quant Time: Mar 05 06:24:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 05 06:21:29 2020
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	278611	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1136849	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	727201	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1556344	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1547511	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1777063	20.00	ng/ul	-0.01

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.17	96	6896	1.06	ng/uL	0.00
5) Phenol-d5	6.82	99	118712	5.59	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	72874	6.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	107081	5.82	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	89489	5.12	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	45932	5.26	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	45578	4.64	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	101989	5.39	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	129067	6.22	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	339982	6.18	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	395924	6.02	ng/ul	0.00
52) 4-Nitrophenol-d4	14.49	143	19293	1.83	ng/ul	0.00
58) Fluorene-d10	15.27	176	314900	6.61	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	17952	2.09	ng/ul	0.00
71) Anthracene-d10	17.12	188	480365	6.87	ng/ul	0.00
79) Pyrene-d10	19.37	212	624351	7.71	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	680934	7.49	ng/ul	-0.01


Target Compounds					Qvalue	
45) Dimethylphthalate	13.73	163	64968	1.144	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : BP002060.D
Acq On : 04 Mar 2020 20:50
Operator : CG/JU
Sample : L1677-19
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CB6

Quant Time: Mar 05 06:24:08 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 05 06:21:29 2020
Response via : Initial Calibration

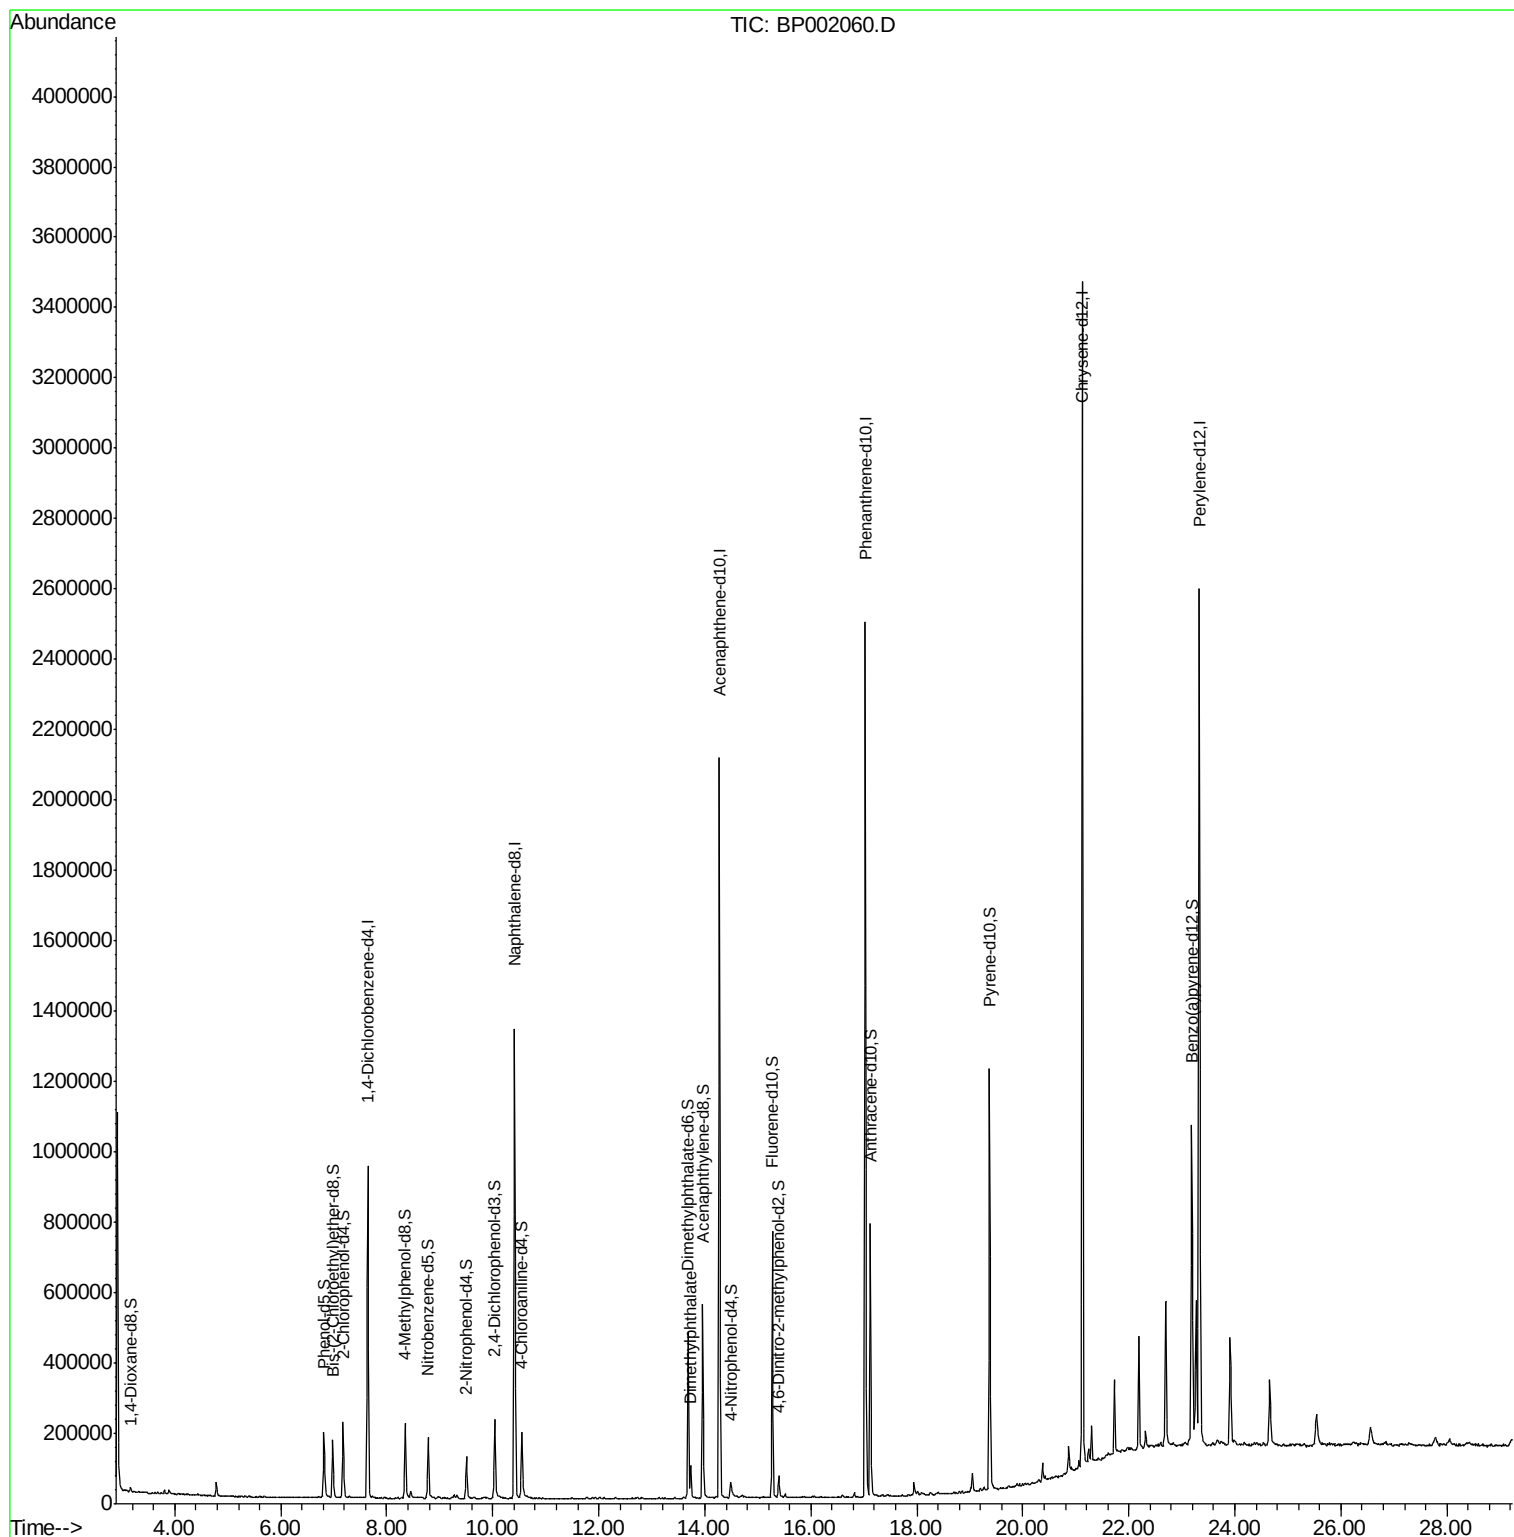

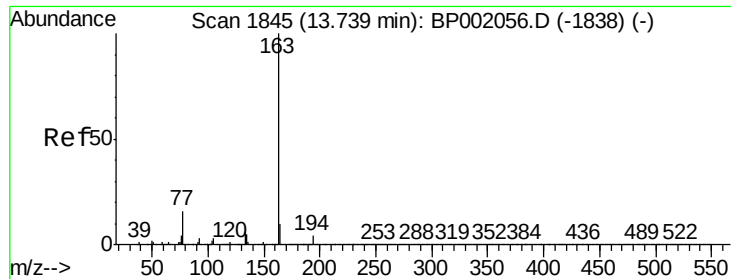

#45

Dimethylphthalate

Concen: 1.144 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BP002060.D

Acq: 04 Mar 2020 20:50

Instrument :

BNA_P

ClientSampleId :

C0CB6

Tgt Ion:163 Resp: 64968

Ion Ratio Lower Upper

163 100

194 4.0 3.6 5.4

164 9.7 8.2 12.4

