

Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP030420\
 Data File : BP002054.D
 Acq On : 04 Mar 2020 17:01
 Operator : CG/JU
 Sample : L1677-09
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0CB9

Quant Time: Mar 05 05:50:13 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 03 05:31:15 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.64	152	276281	20.00	ng/ul	0.00
18) Naphthalene-d8	10.41	136	1138648	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.27	164	718105	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.03	188	1531864	20.00	ng/ul	0.00
78) Chrysene-d12	21.12	240	1519786	20.00	ng/ul	0.00
86) Perylene-d12	23.33	264	1739177	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.16	96	11917	1.85	ng/uL	0.00
5) Phenol-d5	6.82	99	202232	9.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	6.98	67	120737	10.82	ng/ul	0.00
9) 2-Chlorophenol-d4	7.18	132	186302	10.22	ng/ul	0.00
13) 4-Methylphenol-d8	8.35	113	164297	9.49	ng/ul	0.00
19) Nitrobenzene-d5	8.78	128	81483	9.32	ng/ul	0.00
22) 2-Nitrophenol-d4	9.50	143	83921	8.53	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.04	165	178497	9.42	ng/ul	0.00
29) 4-Chloroaniline-d4	10.55	131	230679	11.10	ng/ul	0.00
44) Dimethylphthalate-d6	13.69	166	582147	10.71	ng/ul	0.00
47) Acenaphthylene-d8	13.96	160	682333	10.50	ng/ul	0.00
52) 4-Nitrophenol-d4	14.48	143	39852	3.84	ng/ul	0.00
58) Fluorene-d10	15.27	176	525725	11.18	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.39	200	36106	4.28	ng/ul	0.00
71) Anthracene-d10	17.12	188	803685	11.67	ng/ul	0.00
79) Pyrene-d10	19.37	212	980696	12.33	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.19	264	1074064	12.07	ng/ul	0.00
Target Compounds						
45) Dimethylphthalate	13.73	163	210418	3.751	ng/ul	99
77) Fluoranthene	19.05	202	100763	1.035	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA P\DATA\BP030420\
Data File : BP002054.D
Acq On : 04 Mar 2020 17:01
Operator : CG/JU
Sample : L1677-09
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0CB9

Quant Time: Mar 05 05:50:13 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\SOM-EPA-BP022720MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 03 05:31:15 2020
Response via : Initial Calibration

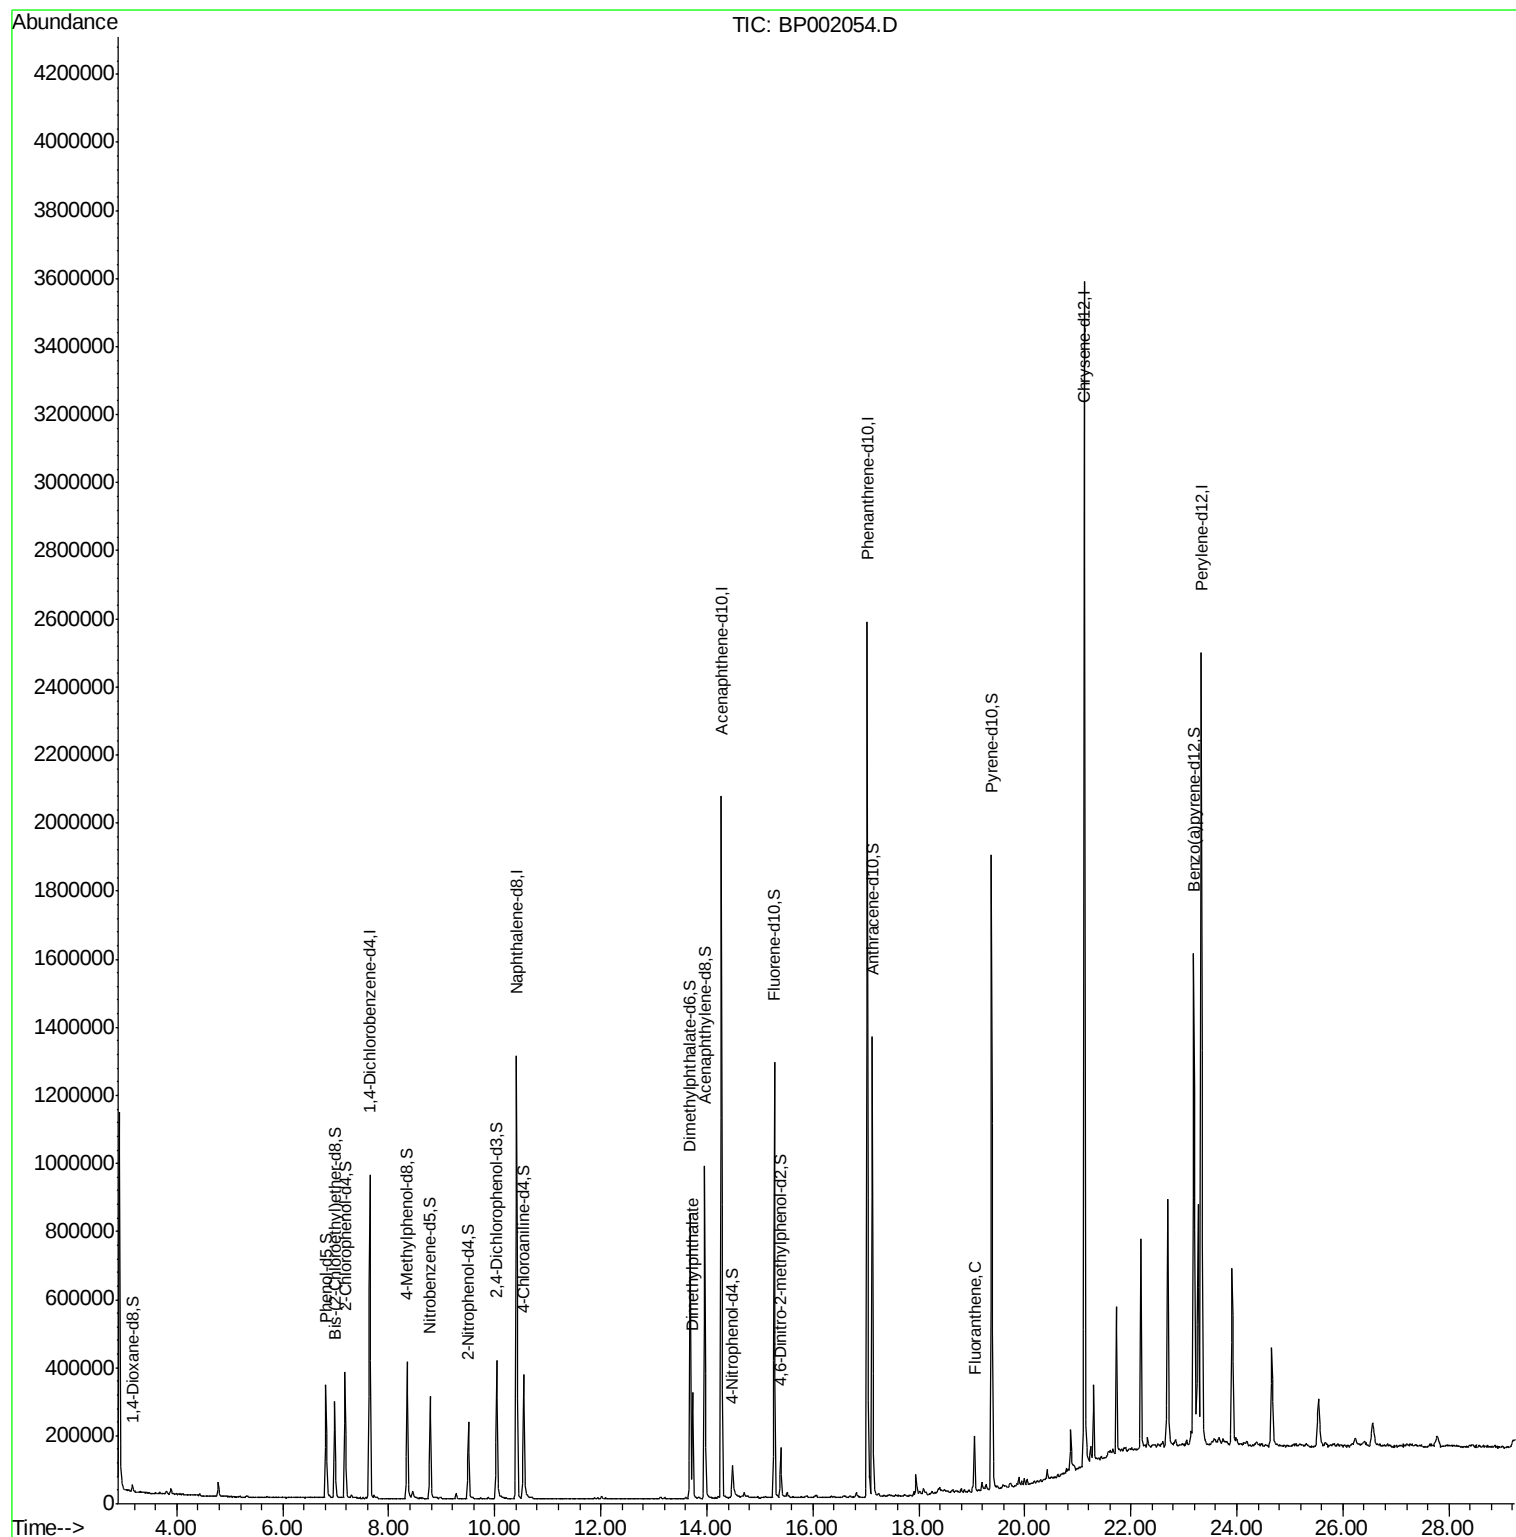

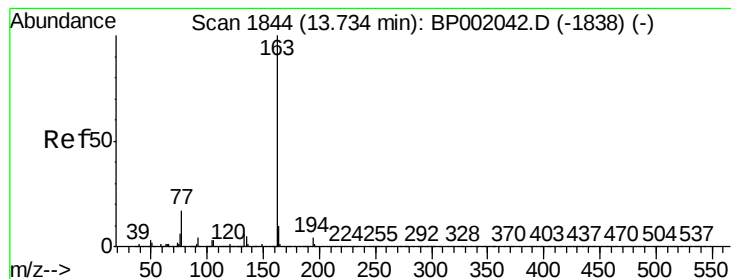

#45

Dimethylphthalate

Concen: 3.751 ng/ul

RT: 13.73 min Scan# 1844

Delta R.T. -0.01 min

Lab File: BP002054.D

Acq: 04 Mar 2020 17:01

Instrument :

BNA_P

ClientSampleId :

C0CB9


Tot Ion:163 Resp: 210418

Ion Ratio Lower Upper

163 100

194 4.6 3.6 5.4

164 10.0 8.2 12.4

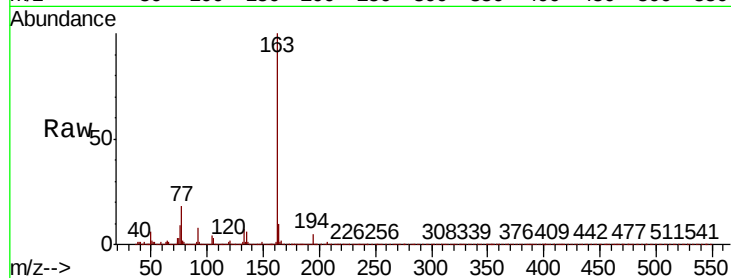



Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

13.73

Time-->

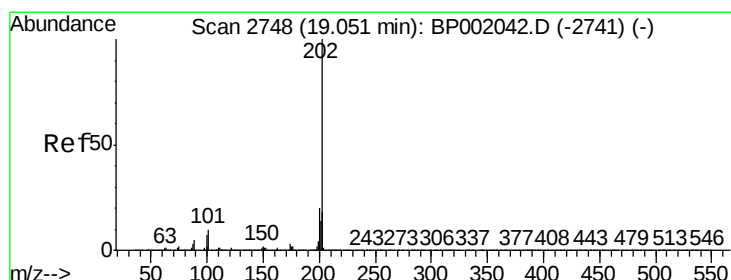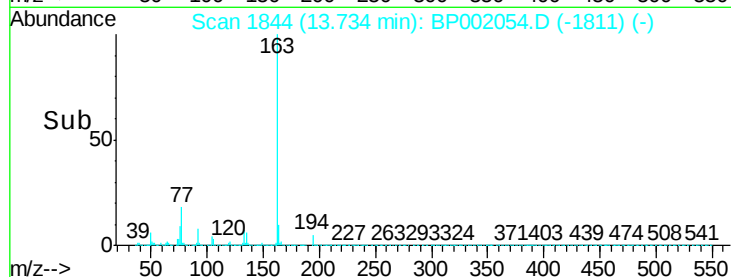

#77

Fluoranthene

Concen: 1.035 ng/ul

RT: 19.05 min Scan# 2748

Delta R.T. 0.00 min

Lab File: BP002054.D

Acq: 04 Mar 2020 17:01


Tgt Ion:202 Resp: 100763

Ion Ratio Lower Upper

202 100

101 8.9 8.2 12.2

100 6.5 6.3 9.5

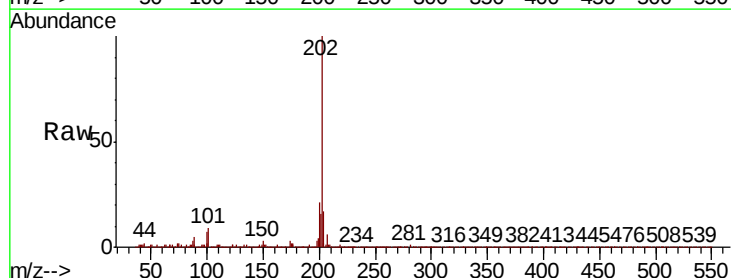

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): E

19.05

Time-->

